



Operation Manual

Microtector II G460

1 to 7-Gas Detector



GfG Products For Increased Safety

Congratulations!

You decided for a high technology product of GfG. A good choice!

Our detectors are characterized by reliability, safety, best performance and economic efficiency.

They comply with national and international directives.

This manual will help you to operate the detector quickly and safely.

Please take note of the operational hints before putting into operation!

For any questions please feel free to contact us.

GfG Gesellschaft für Gerätebau mbH

Klönnestraße 99

D-44143 Dortmund

☎: +49 - 231 - 564 000

Fax: +49 - 231 - 516 313

www.gfg.biz

info@gfg.biz

Content

	Page
INTRODUCTION	5
For your safety	5
Application and purpose	5
Special conditions for safe use	6
Design	6
OPERATIONAL HINTS	7
Switching On and Off	7
Additional Messages during Detector Start	7
Detection Mode	8
Battery Capacity and Battery Alarm	8
Alarms	8
Reset of Alarms	9
STEL, TWA, Peak, Minimum Values	9
Flip-Flop Display, Zoom Display	9
Peak – Display of Peak Values	10
Turn On /Off Lights	10
Display Illumination	10
Storing Measurement Data with the Data Logger	10
Influence of Oxygen and Interfering Gases	11
Special Notes for LEL Monitoring	11
HI%-Measurement of Methane resp. Natural Gas ^[#]	11
Service Mode	11
Main Menu	11
Location – Entering a Location	12
User – Entering User Name	12
Data Logger Settings	12
Signal – Selection of Confidence Bleep	13
AutoCal – AutoCal-Adjustments	13
Options – Anti-Lazy-Battery, Alarm Volume, Display Contrast	14
Tolerance band on/off	14
Service Menu	14
Sensor Menu – Sensor-specific Functions	14
Zeroing – Adjustment of Zeropoint	15
Calibration – Sensitivity Adjustment	16
Alarms – Adjusting the Alarm Thresholds	16
Calibration Data - Date & Status of last calibration	17
Information – Sensor Information	17
Unit and Gas - Selection of Detection Range	17
System Menu – General Settings	18
Bump Test – Date and Interval	18
Calibration (ZERO+CAL) – Date and Interval	18
Inspection – Date of next Inspection	19
Time – Date and Time of the Instrument	19
System Options – Language, Vibration and Latching Alarm, SD Card Check, Auto Save	19
Sensor Selection – Activation / Deactivation	20
AutoCal-Air – Sensor Release for AutoCal Adjustments	20
AutoCal-Gas – Sensor Release for AutoCal Adjustments	20
Information – Detector, Firmware Version, Serial Number, Supply Module	20

Charging of Rechargeable Battery Pack **20**

Lazy-Battery-Effect on NiMH Battery Packs and its Clearance 21

Replacement of Alkaline or Rechargeable Batteries 22

ANNEX **22**

Cleaning 22

Maintenance and Inspection 22

Service - Repair 22

Calibration Accessories 23

Test with Docking Station DS400 23

Trouble Shooting 23

Accessories and Spare Parts 25

Hints for a non-polluting disposal of old parts 26

Sensor Types and Detection Ranges 26

Sensor Specification 27

Alarm Thresholds – Standard Setpoints 32

Technical Data 33

EC-Type Examination Certificate 35

Introduction

For your safety

According to § 3 of the law about technical working media and consumer products for Germany according to "Geräte- und Produktsicherheitsgesetz (GPSG) this manual points out the proper use of the product and serves to prevent dangers. It must be read and adhered to by all persons who use, service, maintain and check this product. This detector can do the job designed to do only, if it is used, serviced, maintained and checked according to the instructions given by GfG Gesellschaft fuer Geraetebau. The warranties made by GfG with respect to the product are voided, if the product is not used, serviced, maintained and checked in accordance with GfG's instructions. The above does not alter statements regarding warranties and liabilities in GfG's general conditions of sale and delivery. Repairs must only be done by skilled personnel resp. by trained persons. Modifications and changes of the product require GfG's permission. Unauthorized modification of the product results in the exclusion of any liability for possible damage. Make sure that only genuine GfG accessories are used with the product. Repairs require the use of spare parts released by GfG.

Application and purpose

The G460 is a handheld detector for personal protection from hazards occurring by toxic or explosive gases and vapors and also by a lack of oxygen or oxygen surplus. The detector measures permanently in diffusion mode and gives a visual and audible alarm, if a gas-induced danger builds up. The G460 is approved for the use in explosion endangered areas and is subject to an EC-Type Examination Certificate issued by DEKRA EXAM GmbH, according to directive 2014/34/EU:

Certificate:	BVS 06 ATEX E 017 X		
Labelling:	⊕ II 2G	Ex ia de IIC T4 Gb	-20°C ≤ Ta ≤ +50°C (NiMH-II)
		Ex ia de IIC T3 Gb	-20°C ≤ Ta ≤ +50°C (NiMH)
		Ex ia de IIC T4/T3 Gb	-20°C ≤ Ta ≤ +45°/+50°C (Alkaline)
Labelling:	⊕ I M1	Ex ia I M	-20°C ≤ Ta ≤ +50°C (NiMH-II, NiMH)

The temperature class of the detector in group II depends on the supply module used. When using the „NiMH-II“ accumulator, temperature class T4 is valid for ambient temperatures of -20°C to +50°C, while temperature class T3 is valid when using the „NiMH“ accumulator. Both supply modules are identified by a black enclosure with an inside label showing the type and temperature class. When using the Alkaline batteries (grey housing), temperature class T4 is valid for ambient temperatures from -20°C to +45°C resp. temperature class T3 for ambient temperatures of -20°C to +50°C.

For the use in group I it is only allowed to use the „NiMH“ or „NiMH-II“ accumulator. The detector is valid for ambient temperatures of -20°C to +50°C.

For the use in explosion endangered areas with a measurement function for the explosion protection there is a supplement for the G460 to the above mentioned EC-Type Examination Certificate of DEKRA EXAM GmbH according to guideline 2014/34/EU. Basis of the test were the standards DIN EN 60079-29-1 „Gas detection instruments – requirements to the operational behavior of instruments for the measurement of combustible gases“ and DIN EN 50271 “Electronic instruments for the detection and measurement of combustible gases, toxic gases or oxygen – requirements and testing for warning instruments, that use software and/or digital technology“. Furthermore the G460 was examined on its measurement ability by DEKRA EXAM GmbH on the basis of the standards DIN EN 50104 “Electronic instruments for the detection and measurement of oxygen – requirements to the operational behavior and testing method“ and DIN EN 45544-1/-2 “Electronic instruments for the direct detection and direct measurement of the concentration of toxic gases and vapours part 1: common requirements and testing methods“ and part 2: requirements to the operational behavior of instruments for the measurement of concentration in threshold ranges“. This is approved by the relevant Type Examination Certificate with the number PFG 09 G 001.

The tests of the measuring function contain following sensors and detection ranges:		
EC-Type Examination Certificate BVS 06 ATEX E 017 X (4. and 7. supplement)	MK211-8 MK211-6, MK211-7 MK227-5, MK231-5	for 0..5 Vol.% CH ₄ (CC) for 0..100%LEL CH ₄ , C ₃ H ₈ , C ₆ H ₁₄ (CC) for 0..100%LEL C ₃ H ₈ , C ₉ H ₂₀ ^[#] (IR)
Type Examination Certificate PFG 09 G 001	MK224-5, MK231-5 MK344-4, MK369-6 MK427-5 MK429-5	for 0.02..5%Vol CO ₂ (IR) for 2..500ppm, 5..500ppm CO (EC) for 0..25%Vol O ₂ (EC) for 0.2..100ppm H ₂ S (EC)

At [%]: The measuring function for n-nonane was tested in the range of 0..60%LEL.
The functions being marked with [#] were not subject of the test of the measurement function.

Special conditions for safe use

In explosion endangered areas the G460 must be used properly. This means that the detector must be carried at your body and must not be laid down unattended, to prevent an electrostatic charge of the clip. For the use in mine (group I) it is only allowed to use the „NiMH“ or „NiMH-II“ accumulator. In case readings in gas-free environments show a permanent zero-point deviation, a zero-point adjustment is necessary. Especially after a heavy impact stress the zero-points of the sensors have to be checked and optionally re-adjusted. In case the CC sensor shows “over-range” after a stress impact, the alarm has to be reset in fresh air and the zero-point has also to be re-adjusted. If the G460 is operated continuously for more than one day, the instrument should be turned off and on again every 24 hours latest. Within the system option menu the deactivation of the latching alarm is not allowed for the use as a function tested measurement instrument. For functional and Ex-protection reasons only GfG approved micro SD-memory cards must be used (s. chapter “Accessories and Spare Parts”).


Design




Operational Hints

Switching On and Off




Press the right key shortly to switch the G460 on .

To switch the G460 off, press the right key  for approx. 5 seconds. Release the key when the display reads **SWITCH-OFF 0**.

During charging the standard detection mode is automatically switched off and the charging time is displayed.

After switching on the G460 starts a self-test and displays information about the firmware version, the built-in sensors with detection ranges and alarm thresholds and the date of the next inspection. During the self test the visual and audible alarms are triggered like gas alarms.

 V3.16 G460	Self test + Alarm 1 Alarm 2/STEL/TWA Alarm 3	Self test Alarm 1 + Alarm 2/STEL/TWA Alarm 3	Self test Alarm 1 Alarm 2/STEL/TWA + Alarm 3
User: NAME Location: POSITION 12.Feb.2008 09:31:41	Sensor test O ₂ ✓ CH ₄ ✓ H ₂ S ✓ CO ✓	0...300 ppm CO Alarms Alarm 1 30 ppm Alarm 2 60 ppm 15%STEL --- ppm 8h TWA --- ppm	0...300 ppm CO Calibration dates status 01.Nov.2006 ✓
NEXT INSPECTION 06.FEB.2009	ALL SENSORS READY	ALARMS ACTIVE MONITORING	

Alarm thresholds and calibration data are displayed for all sensors connected. Only as an example it is only CO which is being described here. Depending on the status of the sensors, the instrument may provide additional messages, which may have to be confirmed. Please refer to "Additional messages during detector start" for further information.

If you push the left key (**DETECT**), or if you do not hit any key, during the warm-up period, the detector goes to detection mode. By pressing the right key (**ZERO**) the automatic fresh air adjustment is started. When the detector is equipped with an oxygen sensor, its sensitivity is set to the normal 20.9Vol% oxygen which are present in fresh air.


Once the self test is completed, the instrument is ready to use after about one minute. By hitting the middle key readings and messages can be reset.

Additional Messages during Detector Start


When started, the G460 tests the sensors and supervises their adjustment data. For sensors, which were not adjusted yet or whose adjustment is older than one year, the message "Calibration needed!" is displayed. The reduced adjustment interval of used-up sensors might result in the message "Calibration or replacement is needed!". Exhausted sensors are indicated by the message "Replacement needed!", when the detector is started. These messages must be acknowledged by key.

0...300 ppm CO CALIBRATION needed! INFO NEXT OFF	0...300 ppm CO CALIBRATION or replacement needed! INFO NEXT OFF	O ₂ (EC ₃)-Sensor REPLACEMENT in 30 days at the latest needed! NEXT OFF	O ₂ (EC ₃)-Sensor REPLACEMENT needed! NEXT OFF
--	--	--	--

When a docking station is used for instrument check, the G460 may include intervals for bump test and calibration of sensors. The dates for the next bump test or for the next calibration are calculated automatically on the basis of the last check. Depending on what becomes necessary next, the date for the next bump test or for the next calibration will be indicated, when the detector is started. Should the relevant date be exceeded, the G460 indicates this as „overdue“. This message must be acknowledged by key.

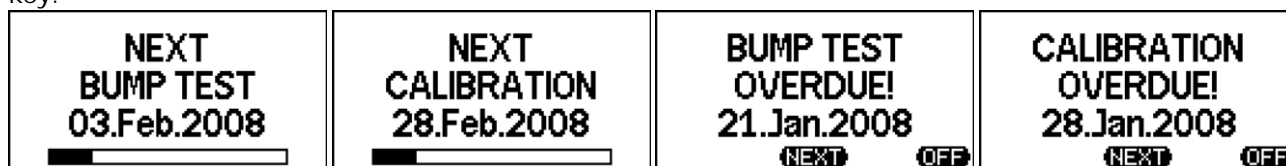

Detection Mode

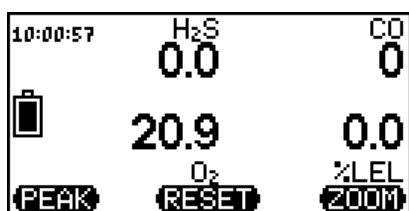

The G460 is ready for operation, if all measurement values, the unit, the gas, the battery capacity and the time are displayed. With more than five measurement values being displayed, the clock will not be shown due to space restrictions. The detector check whether the preset thresholds for the individual gases are exceeded or deviated (O₂).

When more than two measurement values are displayed simultaneously, either the gas type or the unit is shown. By hitting the right key **ZOOM** measurement values can be displayed individually with gas type and unit.

Battery Capacity and Battery Alarm



When in detection mode, the battery capacity can be determined from the battery symbol that is shown on the left of the display. The black bar represents the residual capacity. The residual capacity can also be displayed as a number by pressing the right **ZOOM** button. (*1)

The fully charged battery pack or fresh batteries of the G460 have a capacity (depending on sensor combinations) of approx. 5-170 hours of continuous operation (see technical data). The operational time may be reduced by activated alarms. In the top left corner of the display the remaining battery capacity is indicated by a battery symbol. The black area represents the remaining capacity. If the charging status reaches a low level which is shown as a blank battery symbol, the instrument switches to "energy-saving mode". In this mode the green background illumination will not be activated whenever you hit any key. In case of gas alarms also the red display illumination will not be triggered. The alarm will only be shown by the alarm LEDs and with a maximum volume of 90 db(A). If the charging status sinks even further, battery alarm is given acoustically. In this status the battery symbol flashes. The maximum remaining term is displayed every minute. After 15 minutes the instruments automatically shuts off with a clear acoustic signal. The display reads "OFF" for 5 minutes. Selecting the "Anti-Lazy-Battery" within the option menu the instrument does not automatically shut off after 15 minutes but when falling below a minimum voltage.

To (*1): When using the NiMH F25 or NiMH-II A21 power pack, there can especially be an elevated residual capacity shown if relatively new batteries are being used. In extreme cases, a full battery can be indicated during half of the life. The residual capacity display then falls considerably faster. This normalises itself the older the batter becomes or in relation to the number of charging/discharging cycles. The battery alarm is triggered in good time however, irrespective of this.

Alarms

Should the measured gas concentration exceed a pre-set threshold, the detector immediately gives an audible and visual alarm. The display indicates which gas has caused the alarm. An extremely loud acoustic alarm (103 dB(A) at 30 cm) and bright flashing alarm LEDs provide reliable warning for dangerous gas concentrations. In case of a gas alarm the colour of the whole display turns into orange or red depending on the alarm status. The G460 provides up to three alarm modes. The LO-alarm AL1 can be reset, while the HI-alarms AL2 and AL3 are latching (default). There are three alarm levels for oxygen and combustible gases


(e.g. CH₄), and two thresholds for toxic gases (CO, H₂S). For toxic gases the G460 provides additional alarms for exceeding of short term exposure level (STEL) and time weighted average (TWA). For further information see "Alarm Thresholds – Standard Setpoints" and "Alarms – Adjusting the Alarm Thresholds". The alarm can also be triggered in combination with a vibration alarm, if the instrument provides a relevant "battery pack with integrated vibrator".

Kind of alarm	Sensors	Number of Alarms	Description
Instantaneous value (AL)	oxygen	3	An instantaneous alarm is activated immediately, if the gas concentration exceeds resp. falls below a pre-set threshold. The alarm thresholds are adjustable.
	combust. gases	3	
	toxic gases	2	
Short term exposure level (STEL)	toxic gases	1	The short term exposure level (STEL) is the average concentration over a period of 15 minutes. The STEL alarm is not latching. It resets automatically as soon as the concentration has fallen below the threshold.
Time weighted average (TWA)	toxic gases	1	The time weighted average (TWA) refers to an 8 hours shift and calculates the average concentration. The TWA alarm cannot be reset. It is only de-activated, if the detector is switched off.

The alarms are prioritized as follows: Power fault, overrange, AL3, TWA > AL2, STEL > AL1, underrange > temperature fault.

Reset of Alarms

The latching (default) alarms 2 and 3 can be reset by pressing the **RESET** key, if the gas concentration has fallen below or exceeded (O₂) the pre-set thresholds. Alarm 1 is not latching and resets automatically, when the alarm condition does not exist any longer. If the detection range of the CC sensor (e.g. CH₄) is exceeded, the display additionally reads „OVER RANGE“ instead of the value, for gas concentrations above 110 % LEL. In this case the sensor is deactivated to avoid damage. The alarms and the message "OVER RANGE" remain. This alarm can only be reset by pushing the **RESET** key. Then the display asks:

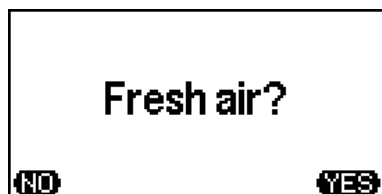

Only if you made sure **that the sensor is not exposed to combustible gas but to fresh air only, you may answer this question with YES**. In this case the sensor turns on again and indicates gas concentrations after a short warm-up time!


For further details please refer to „Special Notes for LEL Monitoring“.

STEL, TWA, Peak, Minimum Values

After switching the detector on, measurement is effected continuously in diffusion mode. In this mode, all concentrations are shown in the display. In addition, short term and long-term averages (STEL and TWA) are calculated for toxic gases, and for non-toxic gases peak and minimum values (MAX and MIN) are stored. The stored values can be read from the display, if you turn to the relevant display mode by means of the right key (**ZOOM**, see below).

Flip-Flop Display, Zoom Display

The display can be turned by 180° by pressing the right and the left key simultaneously and then releasing them. This allows easy reading when carrying the detector on the belt. For activating the zoom display, press the right key (**ZOOM**). Press the key shortly to display one value. Repeated pressing of this key displays the individual measurement values of the individual sensors in zoomed reading one after the other: When a zoomed value is displayed, press **ZOOM** long to change to the following detail reading:

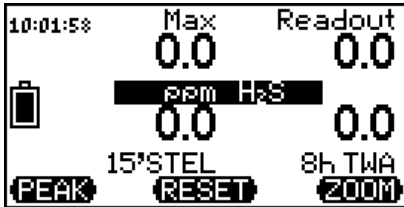


Example of zoom display for H₂S:

- Top left: Peak value
- Top right: Current gas concentration
- Bottom left: STEL value (15 minutes)
- Bottom right: TWA value (8 hours)

Pressing **ZOOM** a certain time changes from one to the other zoom modes. After one zoom mode being activated, the display returns back to normal mode after approx. 10 seconds.

Peak – Display of Peak Values

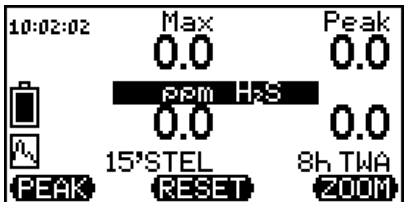

During peak mode (activation by left key **PEAK**) peak values can be monitored and displayed. The display shows an animated symbol in the left bottom corner. Within *zoom display* the peak value will be displayed in the top right corner instead of the actual gas concentration.

Pressing **RESET** during peak mode, the peak memory will be reset to the current gas concentration. Pressing **RESET** during zoom display, the peak memory and the peak value memory will be reset to the current gas concentration. By pressing **PEAK** again, the peak mode is deactivated.

Turn On /Off Lights

The G460 is optionally available with a rechargeable battery pack with lights. The lights can be switched on by keeping the left key pressed for approx. 3 seconds, and turned off by pressing this key shortly. The lights are useful e.g. when the device is linked to a cord and let down into a sewer system. Using the lights can prevent the device from being dipped into water.

Display Illumination

The display illumination is turned on for approx. 10 seconds whenever you hit any key. It turns off automatically after that time. Should the battery or accumulator be almost exhausted, the display illumination cannot be activated any longer.

Storing Measurement Data with the Data Logger

The measurement data can be stored in an integrated data logger or on a detachable micro SD card. A special activation of the data storage is not necessary. With the internal data logger about 1800 events for all measurement values and further information can be stored, containing date, time, location, alarms and special events. Within the main menu under "data logger" different functions of the data storage can be set. It provides a selection of the storage of average values, peak values or instantaneous values as well as the storage interval from 1 second to 60 minutes. The default setting of storing is a loop memory. The oldest event will be overwritten when the data loggers is full. The measurement data of the Microtector II can be read on a PC by means of a charging adaptor, a USB-interface and the GfG-Interface software. The configuration of the data logger can be changed with the interface program. Nearly an unlimited amount of measuring points for all measurement values and other information can be stored on the micro SD card, including date, time, location, user, alarm status, battery status and present device configuration. The measurement data are stored as an average with an interval of one minute resp. five seconds in case of alarm. Two text files are generated each month. The file *M.TEXT contains data from the measurement operation and the file *C.TXT contains data from the charging processes. Depending on the intensity of use and alarms being triggered, the files have a size of about 1-2 MB at the end of the month. With a 1GB micro SD card data can be saved for a theoretic period of more than 40 years. The micro SD card can be removed by switching the instrument off and opening the battery pack. Using an SD-card reader data can be read on a PC or be displayed with a text editor or spreadsheet program. Data can be opened in Excel by using mouse and performing drag & drop. After adjusting the width of the column a diagram of the records can be generated. The micro SD-card must be formatted with a FAT (FAT16) and not with the FAT32 file system.

Influence of Oxygen and Interfering Gases

It is to be considered, that the measurement of gas and/or vapour concentrations in the range below 100% LEL cannot be done accurately, if the oxygen concentration at the same time is below 10 %-Vol.. In this case the CC sensor suffers from a lack of oxygen, which is necessary for the "catalytic combustion". If the oxygen sensor detects such a low concentration, the display reads "?????" instead of the LEL value. When the oxygen concentration exceeds 10 %-Vol., the LEL value will be displayed correctly again. The EX-approval does not cover the use of the detector in oxygen enriched atmospheres. Certain components, known as „sensor or catalyst poisons“, may affect the signal behaviour of the CC sensor. The "sensitivity", i.e. the capability of the sensor to give signals, is reduced. Components of this kind are e.g. sulphuric, lead or silicone compounds.

Special Notes for LEL Monitoring

For LEL monitoring the G460 may use a catalytic combustion (CC) sensor. Due to this principle the G460 cannot distinguish between measurement values in the LEL range and those in the high Vol.-% range (e.g. > 20 Vol.-% CH₄). Concentrations of more than 110 % LEL might also damage this sensor. To prevent such a damage, the sensor is turned off, when gas concentrations of more than 110 % LEL are measured. Only pressing the key **RESET** and confirming the question "Fresh Air?" by means of key **YES** the sensor is turned on again. Oxygen concentrations of less than 10 %-Vol. do not allow the CC sensor to correctly detect combustible gases and vapours. The paragraph „Influence of Oxygen and Interfering Gases“ provides additional information.

HI%-Measurement of Methane resp. Natural Gas^[#]

In standard detection mode methane (CH₄) can be measured within a range of 0..100 %LEL by using either a catalytic combustion sensor (CC) or an infrared sensor (IR). In this mode all gas alarm thresholds are monitored. If the instrument is equipped with a special HI%-IR sensor (MK227-5 or MK231-5), monitoring of higher ranges of up to 100 %-Vol. CH₄ is possible. By pressing the middle and left key simultaneously the mode will be switched to HI%-range. In this mode no gas alarms will be monitored. Apart from deactivated gas alarms also the confidence bleep and optionally the catalytic combustion sensor are deactivated. The display shows in the left top corner the **HI%**-symbol. The measurement value of the infrared sensor is shown in %-Vol. CH₄ and the position for the measurement values of the catalytic combustion sensor remains blank. The pressure dependence of the IR sensor explained within the "Sensor Specifications" must be noticed. If the gas concentration falls below 5 %-Vol. CH₄ the %LEL range can be re-activated by hitting the middle and left key simultaneously. Gas alarm, confidence bleep and optionally catalytic combustion sensor are re-activated as well.

Service Mode


Press the middle key (**RESET**) for approx. 5 seconds to activate the service mode. In the service mode the G460 can be adjusted by changing of program parameters. Certain menu points require the access code „0011“ to prevent accidental change of important functions by unauthorized persons. During the service mode all alarms are deactivated. The main menu is the first menu point in the service mode.

Main Menu

The menu points of the main menu are:

1. **Location** (= Entering a location)
2. **User** (= Entering of identity)
3. **Data logger** (= Adjustment of data logger functions)
4. **Signal** (= Setting of confidence bleep intervals)
5. **Service** (= Starting the service menu)
6. **AutoCal** (= AutoCal adjustment with fresh air or with test gas)
7. **Options** (= Anti-Lazy-Battery, contrast, alarm volume)
8. **Pump** (= Information and status of the pump)

Menu control: The function of the key is explained by the display reading above the relevant key.

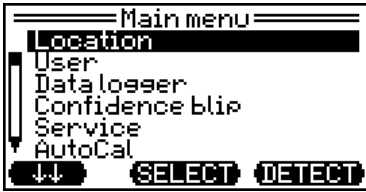

- Left key (↓) = Scroll down
- Middle key (SELECT) = Selection of marked menu point
- Right key (DETECT) = Back to detection mode

Location – Entering a Location

From a deposited table one location out of hundred possible locations can be selected. The first two digits stand for the number of the table entry. Except of the table entry “00” all other 99 entries can only be edited by means of a PC. Within the table entry “00” up to 15 letters / figures can be entered, which will be stored as “**Location**” on the G460.

If **Location** is selected by pressing the middle key (SELECT), the following reading is displayed:



During location selection a consecutive number is determined first:

- EDIT = Confirming of consecutive number
- EXIT = Back to main menu
- ↑ = Changing of consecutive number

After confirming the consecutive number by pressing the left key (EDIT), the location entry will follow:

The function of the keys is as follows:



- ABC↓ = Change of symbol – moving forward in alphabetical order
- <> = Enters the blinking letter or figure and moves the cursor to the right
- 012↑ = Change of symbol – moving back in alphabetical order


User – Entering User Name

From a deposited table one out of ten possible entries can be selected. The first two digits stand for the number of the table entry. Except of the table entry “00” all other 9 entries can only be edited by means of a PC. Within the table entry “00” up to 15 letters / figures can be entered, which will be stored as “**IDENTIFICATION**” on the G460. Entry is completed automatically, when the cursor reaches the end mark “>”. Entering the user name (ID) is done in the same way as entering the location.

Data Logger Settings


Within the menu point “**Data Logger**” different settings can be done:

- Full** - Deleting data from data logger (indication of storage occupancy)
- Mode** - Selection of instantaneous, average or peak value
- Interval** - Interval of data recording (adjustable from 1 second to 60 minutes)

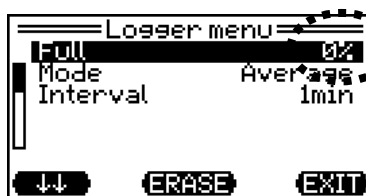


Parameter **Full** shows the occupancy of the data logger.

- ↓ = Scroll down to next parameter
- ERASE = Deletes data. A security check is effected “Delete data?” Confirm with the right key **YES**, resp. deny with the left key **NO**.
- EXIT = Back to main menu

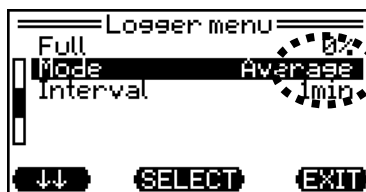

If parameter **Mode** was selected with **SELECT**, instantaneous value, average value or peak value (PEAK) can be chosen. Press **EXIT** to return to the recorder menu. The selected mode will be kept.

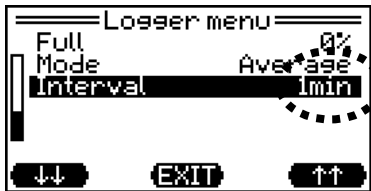


Interval:
The data recording interval can be selected by and between 1 second and 60 minutes.

The recorded data can be read and transmitted to a PC by means of the drop-in charger or the smart charger cap and an optional USB adapter cable.

Signal – Selection of Confidence Bleep

Within the menu point “**Signal**” the interval for releasing the confidence bleep can be chosen in which the G460 triggers a confidence bleep during activated alarm monitoring. Default setting of the interval is 60 seconds.

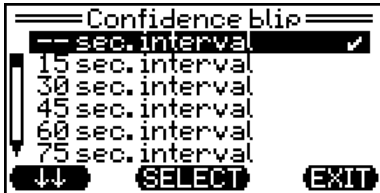

The confidence bleep can be set in intervals of 15 to 90 seconds or be deactivated (enter "--").

- SELECT** = Selection
- EXIT** = Confirm interval and back to main menu
- = Scroll down


AutoCal – AutoCal-Adjustments

Within the menu point AutoCal, several sensors can be calibrated simultaneously with fresh air (ZERO) or test gas (CAL). Normally all sensors except of the CO₂ sensor can be set with fresh air without any further adjustment. For adjustments with test gas the sensors have to be activated according to the test gas / mixture being used (s. chapter “AutoCal Air ...” and “AutoCal Gas ...”). The menu point AutoCal can be selected within the main menu, but is also activated automatically, when the “Smart Cap” or the “Smart Charger Cap” is mounted.





The following functions can be chosen:

- ZERO** = AutoCal with fresh air
- CAL** = AutoCal with test gas
- EXIT** = Back to main menu

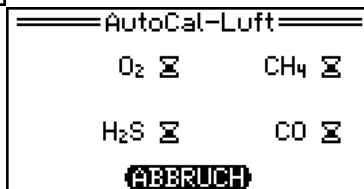

AutoCal adjustment with fresh air successful

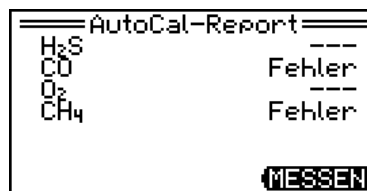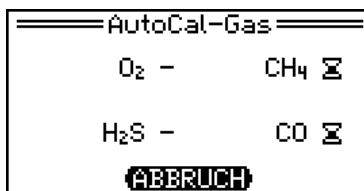

AutoCal adjustment with test gas mixture not successful (e.g. due to wrong test gas concentration)


An AutoCal adjustment with fresh air is only successful, if the measured value does not differ by more than ±10% full scale from the nominal value 0.0 resp. not more than ±5.2 %-Vol. O₂ from the nominal value 20.9 %-Vol. O₂. A successful AutoCal adjustment with test gas is only completed, if the measured value does not differ by more than 25% from the nominal “CalGas” value (see sensor menu “Calibration”). In case of higher deviations the related sensor is marked with “Fault” in the subsequent AutoCal-report. In this case an adjustment with “ZERO” resp. “CAL” or in the docking station is necessary. The adjustment with gas-free fresh air can be done in diffusion mode. Only when zeroing the CO₂ sensor you should not use ambient air, as it always contains a small CO₂ content, which would result in wrong CO₂ measurement values. This is why the zeropoint of the CO₂ sensor should only be adjusted in sensor menu “Zeroing” or in the docking station, using CO₂-free zero gas. This can be e.g. synthetic air, 100 %-Vol. N₂ or specially cleaned air (CO₂-free).

Zero gas (gas-free air) and test gas can be supplied with a volume flow of 0.5 to 0.6 l/min by means of the "Smart Cap" or the "Smart Charger Cap".

Options – Anti-Lazy-Battery, Alarm Volume, Display Contrast

Menu point "Options" allows the following settings:

- When "**Anti-Lazy-Battery**" is activated the level for the automatic shut down due to a nearly discharged battery pack is reduced, i.e. the discharging time of the battery pack is extended. This setting is only active until the instrument is turned off.
- The buzzer volume can be changed to: 103dB(A), 90dB(A) or 0dB(A). For safety reasons, adjustment to 0dB(A) is only possible after entering a service code. During operation a 0dB-symbol is shown in the top left corner of the display. In this case all acoustic signals (gas alarm, fault, battery alarm and confidence beep) are deactivated, so the user has to check the display permanently for possible hazards.
- The display contrast can be changed from 1 = very low up to 15 = very high).

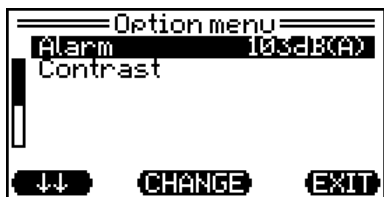

- = scroll down
- CHANGE** = Change selected parameter
- EXIT** = Back to main menu

Tolerance band on/off

In standard detection mode the G460 suppresses small fluctuations around the zeropoints of sensors for toxic and combustible gases. For the oxygen measurement small fluctuations around 20.9 %-Vol. O₂ (fresh air) will be suppressed. The displayed value is kept at 0 until the gas concentration will have reached 200 % of the tolerance band value. This tolerance band is a default setting but can be deactivated: When going to service mode, enter <REAL> for deactivation or <BAND> for activation of the tolerance band instead of the normal access code. For more details about the tolerance band values see chapter "Sensor Types and Detection Ranges".

Service Menu

Enter the service menu by selecting "**Service**". Within the service menu the G460 can be adjusted by changing program parameters. The menu points are only accessible with the code „0011“. The code prevents important functions being changed by mistake or by unauthorised persons. In service mode no alarms can be released.



- ABC** = one letter ahead
- <<>>** = confirms letter (*cursor moves automatically to the next digit*). Holding the key deletes the last entry, the cursor moves one position backwards.
- 012** = one letter

When entering code 0011, the display reads:



Menu point **System** allows performing general adjustments (see section „System Menu“). Within the menu point **Sensors** you can set sensor-specific functions (zeropoint, span). You can also call for information or set alarm thresholds.

Press **DETECT** to leave the service menu and to return to detection mode.

Sensor Menu – Sensor-specific Functions

Following functions refer to individual sensors of the G460. In service menu every sensor can be selected individually. The adjustments are only valid for the selected sensor.

For the following function description of sensor-specific adjustments the CH₄ resp. O₂ sensor is being mentioned as an example. The adjustment possibilities, however, are also valid for the other sensors.




Entering possibilities:
 ↓↓ = Move to next sensor
 SELECT = Select sensor
 EXIT = Back to service menu



For every sensor following adjustments can be done:
Zero (= Zeropoint adjustment)
Calibrate (= Sensitivity adjustment)
Alarms (= Adjustment of alarm thresholds)
Calibration dates (= Date & status of last calibration und zeroing)
Information (= Sensor information: MK type, serial number, detection range, temperature range)
Unit and type of gas = Selection of displayed CH4-unit (%LEL/%-Vol.) resp. displayed type of gas
 ↓↓ = Move to next menu point
 SELECT = Select menu point
 EXIT = Back to service menu


Zeroing – Adjustment of Zeropoint

For adjustment of the zeropoint the sensors have to be supplied with gas-free air resp. the carbon dioxide sensor and the oxygen sensor (*1) with 100 %Vol nitrogen. The zero gas can be supplied with a flow of 0.5 to 0.6 l/min by means of the "Smart Cap" or "Smart Charger Cap". Select menu point "ZeroGas" to adjust the zeropoint. The display reads:

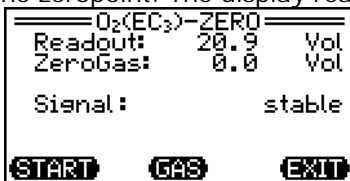

START = Start zeropoint adjustment
 GAS = Enter zero gas concentration
 EXIT = Back to „O₂ menu“

Usually the value for zero gas is 0.0, so this value does not need to be changed. For special applications, however, the zero gas concentration value could be increased slightly after pushing key GAS. After entering **GAS** the display reads:

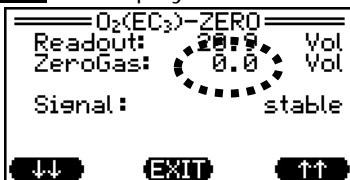

↓↓ = Decrease zero gas value by one unit
 EXIT = Confirm value and back to menu point "ZeroGas"
 ↑↑ = Increase zero gas value by one unit

By entering **START** the zero point adjustment starts:



ABORT = Aborting the adjustment and switching to the CH₄-menu

When the detector measures a constant value, after a stabilization time of 10 seconds, the adjustment is executed and confirmed with "OK". For CC, IR and O₂ sensors the stabilization time is slightly longer but generally limited to 3 minutes.


At (*1): The zeropoint adjustment of the oxygen sensor is done with 100%Vol nitrogen by the manufacturer. For monitoring of the usual alarm thresholds of ≥17%Vol O₂ a readjustment by the user is not necessary. In this case an adjustment of the sensitivity is sufficient.

Calibration – Sensitivity Adjustment

During calibration the gas sensitivity of the sensor is adjusted. Before starting sensitivity calibration, the zeropoint adjustment has to be completed. For a sensitivity calibration a suitable test gas is needed, e.g.


Detection range	Test gas
TOX	Carbon monoxide (CO), Hydrogen sulphide (H ₂ S) or other gases
OX	Fresh air or test gas with 20.9 Vol% oxygen (O ₂) in nitrogen (N ₂)
EX	Methane (CH ₄), Propane (C ₃ H ₈) or other combustible gases (*2)

You can see the recommended test gas from the test report of your G460. For calibration the test gas concentration should be between 30% and 70% of full scale. For IR sensors with measuring ranges >5 Vol.CO₂ the concentration of the test gas must but be between 25% and 75% of the full scale value. The test gas can be supplied by means of the "Smart Cap" or "Smart Charger Cap" with a flow of 0.5...0.6 l/min. For adjusting the sensitivity the sensor menu point „Calibration“ has to be selected.

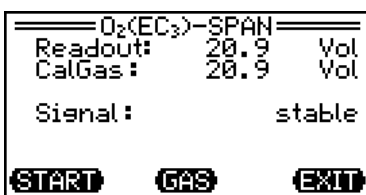


- START** = Start sensitivity calibration
- GAS** = Enter calibration gas concentration
- EXIT** = Back to „O₂ menu“

Entering **GAS** allows to set the test gas concentration within a range of 10...105% full scale:

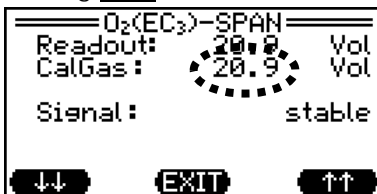

- ↓ = Decreases calibration gas value by one unit
- ↑ = Increases calibration gas value by one unit
- EXIT** = Confirms value and goes back to „O₂ menu“

Entering **Start** starts the sensitivity calibration:

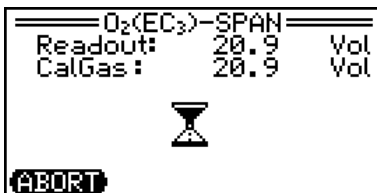

- ABORT** = Stop calibration and back to "O₂" menu


When the detector measures a constant value, after a stabilization time of 25 seconds, the adjustment is executed and confirmed with "OK". Generally the stabilization time is limited to 3 minutes.

At (*2): The sensitivity adjustment of sensors that measure certain combustible gases within LEL-range, e.g. n-hexane, n-nonane or other similar "heavy" vapours, is not uncomplicated. Apart from the availability of such a test gas it is to be considered that when the gas is supplied, the stabilization time may take several minutes. Alternatively the sensitivity adjustment can be performed with a suitable reference gas (e.g. propane). The IR sensor MK227-5, for example, can be supplied with a reference gas of 0.85%-Vol. C₃H₈ (propane) and adjusted to 67%LEL n-hexane or 80%LEL n-nonane. The cross sensitivities for the sensors are described in chapter "Sensor Specifications".

Alarms – Adjusting the Alarm Thresholds


The G460 provides 3 alarm thresholds for each non-toxic gas (O₂, CH₄). For the toxic gases (e.g. H₂S, CO, CO₂) the G460 provides 2 alarm thresholds. The alarms are triggered when the gas concentration exceeds or falls below the threshold. For toxic gases an additional alarm for exceeded long-term (TWA) and short-term (STEL) averages can be activated.

After selecting the sensor menu point **"Alarms"** the following reading is displayed (here: selection of O₂):

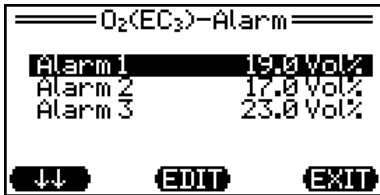

- ↓ = Scroll down
- SELECT = Select menu point
- EXIT = Back to sensor menu

After selecting the alarm thresholds (e.g.: Alarm 1) the value can be entered:

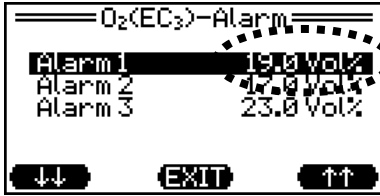


The selected alarm threshold is flashing, the value can be changed now:

- ↓ = Decrease alarm value by one unit
- EXIT = Back to sensor menu
- ↑ = Increase alarm value by one unit


Except for the %LEL detection range all threshold values can be adjusted freely within the detection range or can be deactivated. (0 resp. "----") completely. For %LEL detection ranges the threshold values are adjustable to a maximum of 60%LEL.

Calibration Data - Date & Status of last calibration

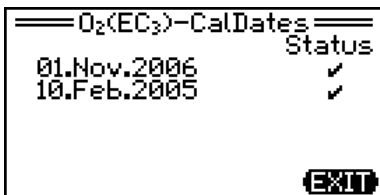

The sensor menu point „CalDates“ indicates the date of the last three sensitivity calibrations and if the calibration was successful (✓) or not (✗).


Information – Sensor Information

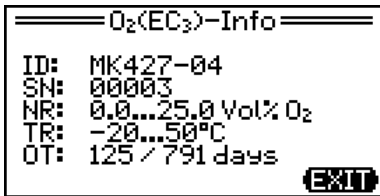

In this menu point specific information for the sensor are displayed:

- ID = Type of sensor
- SN = Serial number
- NR = Nominal detection range
- TR = Temperature range
- OT = Operating time of sensor, e.g. 125 of 791 days

Unit and Gas - Selection of Detection Range

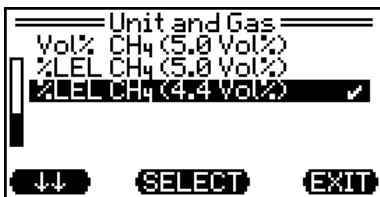


In this menu point you can set the unit for CH₄ to %LEL or %Vol. The volume concentrations in brackets correspond to full scale deflection. This allows to set the detection range to the country-specific LEL value.

When the unit or the gas type were changed, the instrument has to be re-started after the service program has been left, before a bump-test or an AutoCal adjustment in a docking station is performed.

System Menu – General Settings


Selecting „System“ in this menu point, the following reading is displayed:

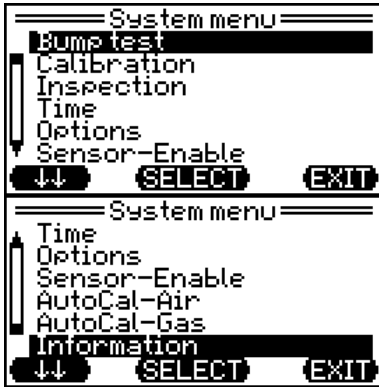

- **Bump test** (status, date of last and next bump test, interval)
- **Calibration** (status, date of last and next calibration, interval)
- **Inspection** (date of next inspection)
- **Time** (date and time)
- **System options** (selection of menu language, vibration alarm on/off, latching alarm on/off, autostore on/off)
- **Sensor selection** (activation resp. de-activation of individual sensors)
- **AutoCal – air** (release of sensors for adjustment with fresh air)
- **AutoCal – gas** (release of sensors for adjustment with test gas)
- **Information** (info about detector type, firmware version, serial number and battery type)

Bump Test – Date and Interval

The bump test (check of sensor values and alarms) can be done easily and quickly by means of the docking station DS400. The bump test is started automatically, the intervals for the bump test are stored in the Microtector II. The bump test interval is activated once the first bump test was done in the docking station.

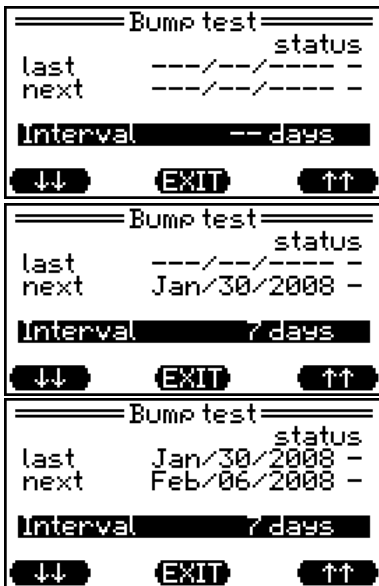


Bump test interval not activated

Bump test interval activated
next bump test required immediately

Bump test on January 30, 2008 was alright
next bump test required in 7 days

Calibration (ZERO+CAL) – Date and Interval

The calibration (adjustment of zeropoint and sensitivity) can easily be done fully automatic with the docking station DS400 very quick and simple. The intervals for calibration are stored in the G460 and activated once the first calibration was done in the docking station.

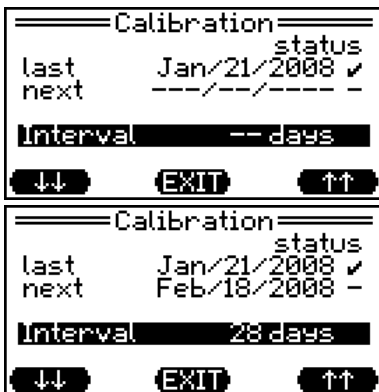

Calibration on January 21, 2008 was alright Calibration interval not activated

Calibration on January 21, 2008 was alright
Next calibration required in 28 days

Inspection – Date of next Inspection

To remind you of the date for the next maintenance resp. inspection, you can enter a date. When it expires, the G460 automatically triggers an alarm. When the entered date is expired, the G460 reports a reminder every time it is switched on.

Select **"Inspection"** in the service menu.



Here the parameter to be changed can be selected (day, month and year).

- EXIT** = Back to system menu
- SELECT** = Select the blinking parameter
- >>** = Move to next parameter




To change a parameter, following options are available:

- ↓** = Decrease value
- EXIT** = Confirm value
- ↑** = Increase value

Time – Date and Time of the Instrument

The instrument provides a clock for the indication of date and time. There is no automatic switching between summer and winter time. This clock is buffered by a lithium cell that is supposed to last for 20 years.

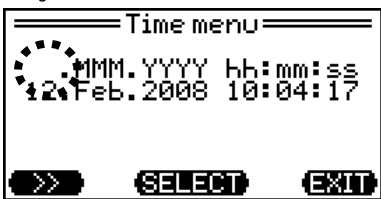

The blinking parameter is chosen by pressing **SELECT**.

With **>>** you move to the next parameter.

With **EXIT** you go back to system menu.




To change a parameter, following options are available:

- ↓** = Decrease value
- EXIT** = Confirm value
- ↑** = Increase value

System Options – Language, Vibration Alarm, Latching Alarm, SD Card Check, Auto Save

The menu point **"System options"** provides information about the selected language, the status of the vibration alarm, the latching alarm function and the autostore function.

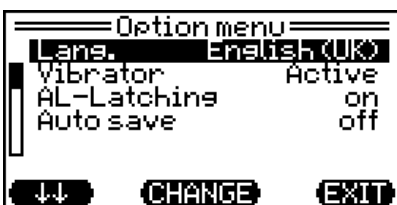


- ↓** = Scroll down
- CHANGE** = Change language resp. vibration alarm
- EXIT** = Back to service menu

All options can be changed. **"Language"** allows to chose German, English (UK), English (US) and French. Under **"Vibrator"** (if available in the battery pack) you can turn the vibration alarm on or off. **"AL-Latching"** determines whether gas alarms 2 and 3 can only be reset by pressing the RESET key or whether these alarms reset automatically as soon as the gas concentration has fallen below the thresholds The deactivation of latching alarms is not allowed for the use as a function tested instrument. In **"SD-card check"** you can select, if the presence of a SD card and the relevant measurement data storage is to be monitored. **"Auto save"** selects whether leaving the service mode saves all changes automatically or whether saving the changes must be confirmed by keystroke.

Sensor Selection – Activation / Deactivation

Every sensor can individually be activated or de-activated. This function is necessary for applications, in which a gas does not need to be measured or if a sensor is to be taken out and not being replaced.

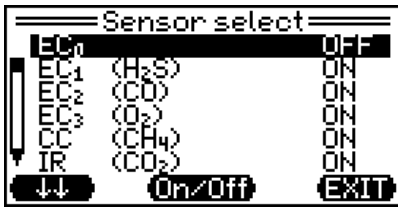

On = Sensor active

Off = Sensor inactive


If the display does not indicate a (Gas), this means that the sensor is not available or is not recognized.

↓ = Scroll down to next sensor

On/Off = Activation / De-activation of sensor

EXIT = Back to service menu

AutoCal-Air – Sensor Release for AutoCal Adjustments

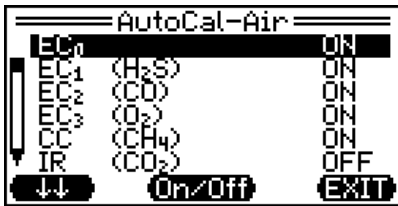


Determination of sensors for which the automatic adjustment with fresh air is possible. Except of the IR sensor for CO₂, all sensors show "ON" and are enabled for automatic calibration with fresh air.

↓ = Scroll down to next sensor

On/Off = Calibration/non-calibration of sensor in AutoCal program

EXIT = Back to service menu

AutoCal-Gas – Sensor Release for AutoCal Adjustments

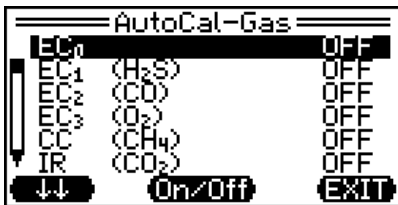

Determination of sensors for which the automatic adjustment with test gas is possible. Generally all sensors show "Off". Should several sensors be calibrated simultaneously with a test gas mixture, you can select these sensors.


↓ = Scroll down to next sensor

On/Off = Calibration/non-calibration of sensor in AutoCal program

EXIT = Back to service menu

Information – Detector, Firmware Version, Serial Number, Supply Module

In the system menu point "Information" you gain information about the detector type, the firmware version, the serial number of the detector, and the type of supply module.

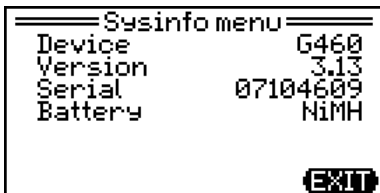

EXIT = Back to service menu

Charging of Rechargeable Battery Pack

Caution: The detector must not be charged in hazardous locations.
The charge contacts must be kept clean (s. chapter "Cleaning").

The rechargeable battery pack in the G460 can be recharged by means of the **drop-in charger (charger tray)**. There are two versions available, one with and one without fixing straps. The version with straps may also be fixed at the wall.

The charger tray is being supplied either by a plug-in mains adapter or by a car charging cable. The charger tray limits the charging voltage for the G460 to max. 6V. The charging process is divided into quick and trickle charge mode. The green LED indicates that the charger tray is ready for operation. The yellow LED indicates the charging mode (off: no detector in charger tray; lit permanently: quick charge; flashing: trickle charge).

When the rechargeable battery pack is completely exhausted, the quick charge mode takes approx. 6...7 hours. Then the charger tray automatically turns to trickle charge, so it is not possible to overcharge the battery pack. Both charging modes are indicated in the display of the G460. When the charger turns to trickle charge, the battery pack has reached at least 90 % of its



Charger tray with bracket

capacity. To reach 100% capacity, you should allow another 2 hours in trickle charge mode. With an optional USB adapter cable, the charger tray allows to download the data from the G460 data logger and to transfer them to a PC.

Alternatively the rechargeable battery pack module in the G460 can be charged with the **Smart Charger Cap**. The Smart Charger Cap is to be fixed to the G460 by means of two knurled screws.

The Smart Charger Cap is also supplied by a plug-in mains adapter or by a car charging cable. The Smart Charger Cap limits the charging voltage for the G460 to max. 6V. The charging process and the signals from the green and yellow LEDs are identical to what was described for the charger tray. The Smart Charger Cap and an optional USB adapter cable also allow to download data from the G460 data logger and to transfer them to a PC.

The Smart Charger Cap also allows to re-calibrate the detector (see picture at right). This cannot be done, however, during charging.

To maintain the full capacity of the battery pack permanently, it is important to make sure that the drop-in charger is only used for charging the battery pack, depending on the operational time and frequency, but not as a depository of the instrument for weeks. The following table shows recommendations for charging the battery pack depending on the frequency of use:



Smart Charger Cap

	Detector used	Charging recommendation
1.	More than 3h a day	Charge after use
2.	Less than 3h a day	Charge every 2. or 3. day
3.	1x per week	Charge 1 day before next use
4.	1x per month; more than 3h	Charge after use as well as 1 day before next use
5.	1x per month; less than 3h	Charge 1 day before next use
6.	1x per quarter or less	Charge after use as well as 2 days before next use

At 4., 5., 6.: If the instrument is only used occasionally, the battery pack should be charged after each use, because parts of the sensor electronics have to be provided with energy even when power is off. In case the instrument was not used for a long time and the battery pack is discharged completely, the instrument should be charged about 2 days before the next use. Possibly the battery pack will then be charged for a short time only (e.g. 11min) in the quick charge mode, switching to trickle charge mode afterwards. A normally discharged battery pack will be charged to 90% of its normal capacity in about 6 to 7 hours in quick charge mode. After another 2 hours in trickle charge mode the battery pack reaches 100% of its normal capacity. In case you do not get the normal operational time from a fully charged battery pack, this may be caused by the "Lazy-Battery-Effect". This effect changes the discharging behavior in a way that despite of a fully charged battery pack the battery indication quickly shows an empty symbol, although the instrument can still be operated for a long time.

Lazy-Battery-Effect on NiMH Battery Packs and its Clearance

Due to temperatures above 50°C, inappropriate use or incorrect charging the NiMH battery packs may become subject to the so-called "Lazy-Battery-Effect", which reduces the operational time of the detector. This can happen, if the detector never discharges the battery pack completely, or if the battery pack is charged too often or for too long. You should avoid, therefore, to start several charging processes a day, or to permanently leave the detector in the charger for several days or weeks.

The "Lazy-Battery-Effect" issue can in most cases be solved by discharging the NiMH battery pack completely. This is why from firmware version 3.23 the menu point "Anti-Lazy-Battery" was added within the "Main Menu/Options". With this function activated, the instrument works as usual. For discharging the battery pack completely, however, the detector should not be switched off manually. The "Anti-Lazy-Battery" option reduces the threshold for the automatic switch off unrecurringly, so the instrument will remain activated after the 15min battery alarm, until a minimum voltage is reached. The battery alarm will still be given every minute, and the

remaining operational time will be displayed in minutes with negative sign. In case of a strong "Lazy-Battery-Effect" it is recommended that this option is repeatedly activated after charging the battery pack.

Replacement of Alkaline or Rechargeable Batteries

Caution: The detector must not be opened in hazardous areas, i.e. the alkaline resp. rechargeable battery pack module must not be changed in such locations.

Turn the detector off before you replace the alkaline or rechargeable battery pack module. For replacing the supply module unscrew the two screws at the front of the detector and pull the complete module backwards, or push it backwards through one of the screw holes. The reverse of the casing holds an Allen key for these screws.

For replacing the alkaline batteries in the battery module use a thin subject to push the two battery cells out through the PCB holes. Take care of the correct polarity when fitting the new 1.5V AA batteries (see battery holder). These batteries have always to be purchased from GfG as the manufacturer of the detector. Internal controls ensure the exclusive use of batteries which comply with the EC-Type Examination Certificate.

The correct battery type is:

DURACELL PROCELL MN1500 LR6 AA or INDUSTRIAL^{BY} DURACELL ID1500 AA (LR6).

The AA battery module or a new rechargeable battery pack module can now be fit. Fix the new supply module by means of the two screws.

Annex

Cleaning

Polluted enclosures can be cleaned with a damp cloth. Do not use solvents and detergents! It is important to make sure that the external charge contacts of the G460 and the charge contact pins of the charging adapter are kept clean. In case of bad contacts of the charging adapter the NiMH-battery pack will only be charged incompletely or not at all.

Maintenance and Inspection

Maintenance and inspection include a regular check and adjustment of sensitivity and zeropoint. A bump test of the device is necessary as well. Depending on ambient conditions, gas monitoring devices may show a different behaviour. Regardless of maintenance it is important, therefore, to test and, if required, adjust the device before they are used (see DIN EN 60079-29-2 chapter 9.2 as well as, in Germany, BG-Chemistry guidelines T 021 and T 023). This test comprises following checks:

- Visual check for mechanical damages
- Visual check of gas inlets
- Charging status of battery / rechargeable battery pack
- Response to zero gas and test gas and alarm triggering

The response behaviour of oxygen sensors can be checked with appropriate test gas (<18 %-Vol. O₂) in combination with the docking station, the "Smart Cap" or the "Smart Charger Cap". The simplest way of checking the response behaviour is to expose the sensor to slowly exhaled air.

Service - Repair

DIN EN 60079-29-2 "... Gas measuring devices – Selection installation, use and maintenance of devices for measurement of combustible gases and oxygen", DIN EN 45544-4 „... Electrical devices for direct detection and direct concentration measurement of toxic gases and vapours, part 4: Guideline for selection, installation, use and maintenance" as well as the relevant national directives are to be adhered to.

Service, in Germany referring to "Explosion Protection Directives" and „BGR 500, chapter 2.33" (formerly: UVV Gase), comprises maintenance, inspection and repair of gas monitoring devices. Guidelines T 021 and T 023 of BG Chemistry describe proper measures. The function test has to be executed before first operation and at least all 4 months and comprises:

- Status of the zeropoint
- Charging status of the battery
- Pump and diffusion inlet
- Display with zero gas and standard test gas and adjustment, if necessary
- Alarm signal release, e.g. with alarm test gas
- Constantly amplified signal with standard test gas
- Response time

The check must be done by an expert, and the result must be confirmed in writing. Any repair of the G460 must generally be done according to the manufacturer's instructions and with genuine spare parts.

Calibration Accessories

For checking the sensitivity the instrument has to be exposed to test gas. By using the "Smart Cap" or the "Smart Charger Cap" the diffusion inlets can be covered, so the sensors can be supplied with test gas at a flow of 0.5...0.6 l/min.. Alternatively and for certain gases this check can also be done in the docking station DS400.

Attention: Test gases, especially toxic gases, can be hazardous. Make sure that test gases are not inhaled. Workplaces where test gas is used for calibration, should be ventilated sufficiently, depending on the kind of gas, its concentration and amount. In special cases an exhaust resp. a gas drain is recommended. Always adhere to the safety advises on gas bottles and to the safety data sheets of the test gases.

Test with Docking Station DS400

The bump test required by T 021 resp. T023 as well as the adjustment of the Microtector II can be done easily and quickly by means of the docking station DS400. The bump test starts automatically and takes approx. 20 seconds. Adjustment is started by just pushing one button, and is completed within a few minutes. The test result is indicated by a green and a red LED. Detailed values are shown in the display of the detector (bump test report, AutoCal-Air report, AutoCal-Gas report). You do not need a PC for bump test r calibration; all relevant data are automatically stored on a SD card in the docking station. The first bump test of a Microtector II G460 in the docking station can automatically activate the interval for bump test and adjustment. Before using the docking station please read and adhere to the relevant operation manual.



Trouble Shooting

	Fault / Message	Cause	Solution
1.	Alarm LEDs flashing, display off	Insufficient supply voltage	Charge resp. replace battery pack
		Hardware or program sequence fault	Call GfG service
2.	"Bootloader" shown permanently with red display illumination	Program memory fault	Transfer firmware to the device or call GfG service
3.	"FAULT! RAM"	RAM fault	Switch device off and on or call GfG service
4.	"FAULT! EEP"	Device parameter memory fault	
5.	"FAULT! BAT"	Battery voltage measurement fault	
6.	"FAULT! ALG"	Program sequence fault / Algorithm	
7.	"Clock chip does not work!" "Time set back to ..."	Hardware fault	Reset message, set clock or call GfG service
8.	"Time set back to ..."	Clock not set or buffer battery empty	Reset message, set clock or call GfG service

9.	"Sensor defect!"	Sensor faulty or not available	Switch device off and on or call GfG service
10.	"Data faulty!"	Sensor data fault	Switch device off and on or call GfG service
11.	"Put sensor in EC1!"	EC sensor in wrong slot	Open device, correct sensor position, then close device
12.	"Put sensor to EC2 or EC3!"		
13.	"Sensor not existing. Deactivate sensor in system menu!"	Sensor not present	Reset message, deactivate sensor in system menu or call GfG service
14.	"Check alarms!"	Sensor was replaced by another type	Check and if necessary change alarm setting in service menu
15.	"Gas not supported!"	Kind of gas not supported or old firmware version	Remove sensor or perform firmware update
16.	"SD card not existing!"	No SD card in the slot	Insert SD card or deactivate "SD-Card check" in service menu
17.	"SD card faulty!"	No SD card in the slot or error when writing data	Reset message or restart device or change card
18.	"No sensors!"	No sensor activated in service menu	Activate available sensor in service menu
19.	Gas indication "START" ("STRT")	Sensor still in start up phase	Wait several seconds
20.	Gas indication "????"	Detection with CC sensor not possible due to oxygen indication <10%Vol	If occurring in fresh air adjust or replace the oxygen sensor
21.	Gas indication "----" / "ERROR"	No gas indication due to faulty sensor or sensor data	Deactivate sensor in service menu or call GfG
22.	Gas indication "UNDER" or "UNDER RANGE"	Massive under-run of detection range	Adjust zeropoint
23.	Gas indication "OVER" or "OVER RANGE"	Gas concentration too high or high cross sensitivity (EC sensors) or activated protective circuit (CC sensors)	Leave the high gas concentration area and reset message for CC sensor and confirm in fresh air atmosphere
24.	Gas indication "FAULT" ("FLT")	IR sensor signal faulty	If occurring repeatedly, call GfG service
25.	Gas indication "TEMP" or "TEMP ERROR"	Sensor operated out of specified temperature range or hardware defect at 0°C<Ta<30°C	Return to normal temperature range or call GfG service
26.	Gas indication "POWER" or "POWER ERROR"	Power supply of sensor is interrupted	If occurring repeatedly, call GfG service
27.	Gas indication "P+T"	see gas indication "TEMP" and "POWER"	see above
28.	"Gas concentration too high!"	Gas concentration still above 5%Vol when changing from HI% range top %LEL range	Wait until gas concentration has fallen below 5%Vol and repeat range change
29.	"Remove charger!"	Alkaline batteries not rechargeable	Disconnect device from

			charger
30.	"Remove battery pack!"	Instrument cannot be switched off due to hardware defect	Remove battery pack from device or call GfG
31.	"No sensors for AutoCal-Air (Gas) enabled!"	No sensors enabled for automatic fresh air resp. test gas adjustment	Enable sensor(s) for automatic adjustment in service menu
32.	"Zero failure – measurement value too high!" (too low)	Possibly gas present or too positive (negative) zeropoint deviation	Adjust zeropoint in gas-free environment or call GfG service
33.	"Calibration failure – measurement value too low!" (too high)	Wrong test gas concentration or sensor sensitivity too low (high)	Check test gas and nominal value or call GfG service
34.	"Zero (calibration) failure – signal unseizable!"	Extreme sensor signal deviation or hardware defect	Repeat process or call GfG service
35.	"Storing failure!"	Parameters cannot be saved when leaving service menu	Switch device off and on, then repeat settings in service menu, or call GfG

Accessories and Spare Parts

	Description	Part No.
1.	Alkaline battery pack without batteries ^(#)	1450200
2.	Alkaline battery pack with vibrator without batteries ^(#)	1450202
3.	Alkaline battery (pack of 10) ^(#)	1450204
4.	NiMH-II A21 battery pack	1450206
5.	NiMH-II A21 battery pack with vibrator	1450207
6.	NiMH-II A21 battery pack with lights	1450208
7.	NiMH-II A21 battery pack with vibrator and lights	1450209
8.	NiMH F25 battery pack	1460206
9.	NiMH F25 battery pack with vibrator	1460207
10.	NiMH F25 battery pack with lights	1460208
11.	NiMH F25 battery pack with vibrator and lights	1460209
12.	Smart Charger Cap (charge, calibrate, data transfer)	1450215
13.	Plug-in charger 100-240VAC (EU adapter)	1450216
14.	Charging cable for cars ^(#)	1450218
15.	Drop-in charger G400-DIC1B (with holder for Microtector II) ^[#]	1450220
16.	Drop-in charger G400-DIC2B (with holder for Microtector II and pump) ^[#]	1450224
17.	Smart cap (for calibration only)	1450225
18.	Transportat and storing case (plastic) ^(#)	1450229
19.	USB Interface cable for PC	1450232
20.	Data logger set 1 with GfG interface software for Microtector II	1450233
21.	microSD-card with adaptor	1460200
22.	Pump G400-MP2 with alkaline battery pack ^[#]	1450252
23.	Pump G400-MP2 with NiMH battery pack	1450253
24.	Docking station DS400 with DIC1D for Microtector II ^[#]	1450401
25.	Docking station DS400 with DIC2D for Microtector II and pump ^[#]	1450402
26.	Sensors see segment "Sensor Types and Detection Ranges"	

Spare parts and accessories should be stored at ambient temperatures of 0...30°C. Storage time should not exceed 5 years. Electrochemical sensors should not be stored for more than ½ year. When you store oxygen sensors be aware of the fact that storage reduces the expected lifetime of the sensor. When storing spare sensors make sure that the ambient atmosphere is free of corrosive media and sensor poisons.

For NiMH battery packs a storing time of only one year is applicable. Before storing the battery pack has to be charged completely. If detectors are stored for more than ½ year the battery pack should be removed.

Hints for a non-polluting disposal of old parts

According to §11 of GfG's general terms and conditions the buyer is committed for a non-polluting disposal of the instrument and its components according to §§11, 12 of the ElektroG. On request the parts may be adequately disposed off by GfG in Dortmund.

Sensor Types and Detection Ranges

Slot	Sensor type	Detection range	Gas	Part No.
EC1	MK380-5 [#]	0 ... 500 ppm	CO Carbon monoxide	1460730
		0 ... 100 ppm	H ₂ S Hydrogen sulfide	
EC1	MK353-5 [#]	0 ... 10 ppm	PH ₃ Phosphine	1460742
EC2	MK369-5 [#]	0 ... 300 ppm	CO Carbon monoxide	On request
EC3	MK369-6	0 ... 500 ppm	CO Carbon monoxide	1460751
	MK383-5 [#]	0 ... 25 Vol.-%	O ₂ Oxygen (2 years)	1460793
	MK393-5 [#]	0 ... 200 ppm	NH ₃ Ammonia	On request
	MK396-5 [#]	0 ... 2000 ppm	H ₂ Hydrogen	1460750
	MK399-6 [#]	0 ... 1000 ppm	NH ₃ Ammonia	On request
	MK402-5 [#]	0 ... 1 Vol.-%	H ₂ Hydrogen	1460758
	MK403-5 [#]	0 ... 4 Vol.-%	H ₂ Hydrogen	1460759
	MK404-5 [#]	0 ... 40 ppm	SiH ₄ Silane	1460762
	MK409-5 [#]	0 ... 50 ppm	HCN Hydrogen cyanide	1460755
	MK427-5	0 ... 25 Vol.-%	O ₂ Oxygen (3 years)	1460791
	MK440-5 [#]	0 ... 10 ppm	SO ₂ Sulfur dioxide	1460765
	MK440-6 [#]	0 ... 50 ppm	SO ₂ Sulfur dioxide	1460766
	MK443-5 [#]	0 ... 500 ppm	CO Carbon monoxide	1460747
	MK443-6 [#]	0 ... 2000 ppm	CO Carbon monoxide	1460748
	MK445-5 [#]	0 ... 100 ppm	H ₂ S Hydrogen sulfide	On request
	MK445-6 [#]	0 ... 500 ppm	H ₂ S Hydrogen sulfide	On request
	MK453-5 [#]	0 ... 200 ppm	NH ₃ Ammonia	1460745
	MK454-5 [#]	0 ... 1000 ppm	NH ₃ Ammonia	1460760
EC2 EC3	MK347-5 [#]	0 ... 100 ppm	NO Nitrogen monoxide	1460744
	MK348-5 [#]	0 ... 30 ppm	NO ₂ Nitrogen dioxide	1460738
	MK379-5 [#]	0 ... 20 ppm	C ₂ H ₄ O Ethylene oxide	1460741
	MK390-5 [#]	0 ... 10 ppm	Cl ₂ Chlorine	1460746
	MK392-5 [#]	0 ... 30 ppm	HCl Hydrogen chloride	1460749
PID (EC2)	MK222-2 [#]	0 ... 500 ppm	C ₄ H ₈ Isobutylene	1460703
	MK222-3 [#]	0 ... 2000 ppm	C ₄ H ₈ Isobutylene	1460704
CC (PL)	MK211-6	0 ... 5 Vol.-%	CH ₄ Methane	1460710
		0 ... 100 %LEL	CH ₄ Methane (*2)	
		0 ... 5 Vol.-%	CH ₄ Methane (raised poisoning firmness)	
	MK211-7	0 ... 100 %LEL	CH ₄ Methane (*2) (raised poisoning firmness)	1460711
	MK211-8	0 ... 5 Vol.-%	CH ₄ Methane (Mining implementation)	1460712
		0 ... 100 %LEL	CH ₄ Methane (*2) (Mining implementation)	
IR	MK224-5	0 ... 5 Vol.-%	CO ₂ Carbon dioxide	1460781
		0 ... 25 Vol.-%	CO ₂ Carbon dioxide	1460782
	MK227-5	0 ... 100 %LEL	CH ₄ Methane (*2) s. below	1460770
		0 ... 100 %LEL	CH ₄ Methane (*2) s. below	1460773
		0 ... 100%Vol	CH ₄ Methane	
	MK231-5	0 ... 5 Vol.-%	CO ₂ Carbon dioxide	1460774
0 ... 100%LEL		Combustible gases and vapours (*2)		
0 ... 5 Vol.-%		CO ₂ Carbon dioxide		
	MK231-5	0 ... 100%LEL	Combustible gases and vapours (*2)	1460778
		0 ... 100%Vol	CH ₄ Methane	

at (*1): T-Band = Tolerance band

at (*2): or one of the following combustible gases and vapours

Sensor	Combustible gases and vapours
MK211-6	CH ₄ (Methane), C ₃ H ₈ (Propane), C ₄ H ₁₀ (Butane), C ₅ H ₁₂ (Pentane), C ₆ H ₁₄ (Hexane), H ₂ (Hydrogen), C ₂ H ₂ (Acetylene), C ₂ H ₄ (Ethylene), CH ₄ O (Methanol), C ₂ H ₆ O (Ethanol), C ₃ H ₈ O (Isopropanol), C ₄ H ₁₀ O (n-Butanol), C ₃ H ₆ O (Acetone), C ₃ H ₆ O ₂ (Methylacetate), C ₄ H ₈ O ₂ (Ethylacetate), C ₄ H ₈ O (Methylethylketone MEK), C ₇ H ₈ (Toluene), C ₆ H ₁₂ O (Methylisobutylketone MIBK), C ₇ H ₁₆ (Heptane), C ₉ H ₂₀ (n-Nonane)
MK211-7	CH ₄ (Methane), C ₃ H ₈ (Propane), C ₄ H ₁₀ (Butane), C ₅ H ₁₂ (Pentane), C ₆ H ₁₄ (Hexane), H ₂ (Hydrogen), C ₂ H ₂ (Acetylene), C ₂ H ₄ (Ethylene)
MK211-8	CH ₄ (Methane), C ₃ H ₈ (Propane), C ₂ H ₆ (Ethane), H ₂ (Hydrogen), C ₂ H ₂ (Acetylene), C ₂ H ₄ (Ethylene)
MK227-5 MK231-5	CH ₄ (Methane), C ₃ H ₈ (Propane), C ₆ H ₁₄ (n-Hexane), C ₉ H ₂₀ (n-Nonane), ETF (Ethyl formate)

Sensor Specification

MK211-6 Catalytic combustion sensor for combustible gases and vapours

Detection range:	0.0 .. 100%LEL or 0,00 .. 5,00 Vol% CH ₄			
Resolution/tolerance band:	0,5 / ±2,5%LEL or 0,02 / ±0,14Vol.% CH ₄			
Response time:	t ₅₀ : ≤10 sec	t ₉₀ : ≤20 sec for CH ₄ (Methane)		
	t ₅₀ : ≤12 sec	t ₉₀ : ≤30 sec for C ₃ H ₈ (Propane)		
	t ₅₀ : ≤40 sec	t ₉₀ : ≤175 sec for C ₆ H ₁₄ (n-Hexane)		
Pressure (70)80....120(130) kPa:	max. ±5%LEL of range or ±10(15)% of display (referred to 100 kPa)			
Humidity 0%...95% r.h.:	max. ±7%LEL of range or ±10% of display (referred to 0% r.h. @40°C)			
Temperature -20...+ 55°C:	max. ±5%LEL of range or ±10% of display (referred to 20°C)			
Cross sensitivities ^[#] @ 50%LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	<u>n-Hexane display</u>
	2,00%Vol H ₂	ca.85%LEL	ca.105% LEL	ca.140% LEL (theor.)
	2,20%Vol CH ₄	= 50% LEL	ca.60% LEL	ca.80% LEL
	1,15%Vol C ₂ H ₄	ca.49% LEL	ca. 59%LEL	ca.78% LEL
	0,85%Vol C ₃ H ₈	ca.41% LEL	= 50% LEL	ca.66% LEL
	0,70%Vol C ₄ H ₁₀	ca.37% LEL	ca.44% LEL	ca.58% LEL
	0,55%Vol C ₅ H ₁₂	ca.30% LEL	ca.36% LEL	ca.52% LEL
	0,50%Vol C ₆ H ₁₄	ca.27% LEL	ca.32% LEL	= 50% LEL
	0,45%Vol C ₇ H ₁₆	ca.18% LEL	ca.23% LEL	ca.36% LEL
	0,35%Vol C ₉ H ₂₀	ca.17% LEL	ca.22% LEL	ca.35% LEL
	May vary from sensor to sensor and depend on the gas concentration and on the age of the sensor.			
Expected lifetime:	3 years in clean air			

MK211-7 Catalytic combustion for combustible gases and vapours (with increased poison resistance)

Detection range:	0.0 .. 100%LEL or 0,00 .. 5,00 Vol% CH ₄			
Resolution/tolerance band:	0,5 / ±2,5%LEL or 0,02 / ±0,14Vol.% CH ₄			
Response time:	t ₅₀ : ≤10 sec	t ₉₀ : ≤20 sec for CH ₄ (Methane)		
	t ₅₀ : ≤12 sec	t ₉₀ : ≤30 sec for C ₃ H ₈ (Propane)		
	t ₅₀ : ≤40 sec	t ₉₀ : ≤230 sec for C ₆ H ₁₄ (n-Hexane)		
Pressure (70)80....120(130) kPa:	max. ±5%LEL of range or ±10(15)% of display (referred to 100 kPa)			
Humidity 0%...95% r.h.:	max. ±7%LEL of range or ±10% of display (referred to 0% r.h. @40°C)			
Temperature-20(-10)...(+40)+55°C:	max. ±5(7)%LEL of range or ±10(20)% of display (referred to 20°C)			
Cross sensitivities ^[#] @ 50%LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	<u>n-Hexane display</u>
	2,00%Vol H ₂	ca.85%LEL	ca.105% LEL	ca.140% LEL (theor.)
	2,20%Vol CH ₄	= 50% LEL	ca.60% LEL	ca.80% LEL
	1,15%Vol C ₂ H ₄	ca.49% LEL	ca.59% LEL	ca.78% LEL
	0,85%Vol C ₃ H ₈	ca.41% LEL	= 50% LEL	ca.66% LEL
	0,70%Vol C ₄ H ₁₀	ca.37% LEL	ca.44% LEL	ca.58% LEL
	0,55%Vol C ₅ H ₁₂	ca.30% LEL	ca.36% LEL	ca.52% LEL
	0,50%Vol C ₆ H ₁₄	ca.27% LEL	ca.32% LEL	= 50% LEL
	May vary from sensor to sensor and depend on the gas concentration and on the age of the sensor.			
Expected lifetime:	3 years in clean air			

MK211-8 Catalytic combustion for combustible gases (Mining)

Detection range:	0.0 .. 100%LEL or 0,00 .. 5,00 Vol% CH ₄			
Resolution/tolerance band:	0,5 / ±2,5%LEL or 0,02 / ±0,14Vol.% CH ₄			
Response time:	t ₅₀ : ≤10 sec	t ₉₀ : ≤25 sec for CH ₄ (Methane)		
	t ₅₀ : ≤20 sec	t ₉₀ : ≤60 sec for C ₃ H ₈ (Propane)		
Pressure (70)80....120(130) kPa:	max. ±5%LEL of range or ±10(15)% of display (referred to 100 kPa)			
Humidity 0%...95% r.h.:	max. ±7%LEL of range or ±10% of display (referred to 0% r.h. @40°C)			
Temperature-20(-10)...(+40)+55°C:	max. ±5(7)%LEL of range or ±10(20)% of display (referred to 20°C)			
Cross sensitivities ^[#] @ 50%LEL:	<u>Gas supply</u>	<u>CH₄ display</u>	<u>C₃H₈ display</u>	
	2,00%Vol H ₂	ca.85%LEL	ca.105% LEL	
	2,20%Vol CH ₄	= 50% LEL	ca.60% LEL	
	1,15%Vol C ₂ H ₄	ca.49% LEL	ca.59% LEL	
	1,20%Vol C ₃ H ₈	ca.47% LEL	ca.57% LEL	
	0,85%Vol C ₃ H ₈	ca.41% LEL	= 50% LEL	
	May vary from sensor to sensor and depend on the gas concentration and on the age of the sensor.			
Expected lifetime:	3 years in clean air			

MK222-2/-3 Photo-ionisation sensor for toxic combustible vapours resp. VOC

Detection range:	0..500/2000ppm i-C ₄ H ₈ (Isobutylene) an more			
Resolution	0,1ppm / 0,5ppm			
Tolerance band:	±0,3 ppm / ±1,0ppm			
Response time:	t ₉₀ : <30 s			
Ionisation potential:	10.6 eV			
Cross sensitivities:	Kerosene: approx.250%; C ₈ H ₈ : 250%; C ₇ H ₈ : 190%; C ₆ H ₆ : 190%; Diesel: approx.110; Petrol: approx.90%; C ₃ H ₆ O: 83%; C ₈ H ₁₈ : 45%; C ₇ H ₁₆ : 40%; H ₂ S: 30%; C ₆ H ₁₄ : 22%; NO: 14%; NH ₃ : 11%; C ₅ H ₁₂ : 10%; C ₄ H ₁₀ =0%; C ₃ H ₈ =0%; CH ₄ =0%; H ₂ =0%			
Response factor:	1-Butanol =3,40 1-Propanol =5,70 Acetone =1,20 Ammonia =9,40 Arsine =2,60 Petrol =1,10 Benzol =0,53 Butadiene =0,69 Butylacetat =2,40	Cyclohexane =1,50 Decane =1,60 Diesel fuel 1 =0,90 Diesel fuel 2 =0,75 Diethyl ether =1,20 Ethyl acetate =4,20 Ethyl acrylate =2,30 Ethyl mercaptan =0,60 H ₂ S =3,20	Heptane =2,50 Isobutanol =4,70 Isobutylene =1,00 Isopropanol =5,60 Jet A fuel =0,40 JP5 fuel =0,48 Methyl acetate =7,00 Methyl mercaptan =0,60 n-Hexane =4,50	n-Nonane =1,60 n-Pentane =9,70 NO =7,20 Octane =2,20 Phosphine =2,80 Propylene =1,30 Styrol =0,40 Toluol =0,53 Xylol =0,50
Expected lifetime:	2-3 years in clean Air			

MK224-5/MK231-5 Infrared sensor for carbon dioxide CO₂

Detection range:	0.02 .. 5.0%Vol (15,0Vol.%) (25.0%Vol ^[#]) Zero point drift ≤ 0.04%Vol		
Resolution:	0,01...0,05Vol.% (0,2Vol.%) (0,5Vol.%)		
Response time:	t ₅₀ : ≤ 20 sec	t ₉₀ ≤ 50 sec	t ₁₀ ≤ 50 sec (decay time @ CO ₂)
Pressure	70...130 kPa:	<1.6% of display per 1% pressure change (referred to 100 kPa)	
Humidity	0%...95% r.h.:	max. ±0.01Vol% or ±2% of display (referred to 50% r.h. @ 20°C)	
Temperature	-20...+55°C:	max. ±0.02Vol% or ±10% of display (referred to 20°C)	
Long term stability	per month:	max. ±0.01Vol% or ±2% of display (laboratory conditions)	
Expected lifetime:	6 years		

MK227-5/MK231-5 Infrared sensor for combustible gases and vapours

Detection range:	0 .. 100%LEL (100%Vol CH ₄ ^[#])				
Resolution:	0,2...1,0%LEL (0,01...0,5Vol.% CH ₄)				
Tolerance band:	±1,2%LEL (±0,05Vol.% CH ₄)				
Response time:	t ₅₀ : ≤ 20 sec	t ₉₀ ≤ 45 sec	(@ CH ₄ Methane)		
	t ₅₀ : ≤ 25 sec	t ₉₀ ≤ 66 sec	(@ C ₃ H ₈ Propane)		
	t ₅₀ : ≤ 30 sec	t ₉₀ ≤ 99 sec	(@ C ₆ H ₁₄ n-Hexane)		
	t ₅₀ : ≤ 55 sec	t ₉₀ ≤ 371 sec	(@ C ₉ H ₂₀ n-Nonane)		
Pressure	70...130 kPa:	<1.5% of CH ₄ display per 1% pressure change (referred to 100 kPa)			
		<1.2% of C ₃ H ₈ display per 1% pressure change (referred to 100 kPa)			
Humidity	0%...95% r.h.:	max. ±2%LEL or ±15% of display (referred to 0% r.h. @ 40°C)			
Temperature	-20...+50°C:	max. ±2%LEL or ±10% of C ₃ H ₈ display (referred to 20°C)			
Cross sensitivities ^[#]	@ 50%LEL:	Gas supply	CH ₄ display	C ₃ H ₈ display	n-Hexane display
		0,85Vol% C3H8	ca.145%LEL	= 50%LEL	ca.67%LEL
		1,20Vol% C2H6	ca.138%LEL	ca.48%LEL	ca.65%LEL
		0,70Vol% C4H10	ca.110%LEL	ca.42%LEL	ca.57%LEL
		1,00Vol% C3H8O	ca.97%LEL	ca.39%LEL	ca.53%LEL
		0,50Vol% C6H14	ca.88%LEL	ca.37%LEL	= 50%LEL
		0,55Vol% C5H12	ca.87%LEL	ca.36%LEL	ca.49%LEL
		0,45Vol% C7H16	ca.82%LEL	ca.34%LEL	ca.47%LEL
		1,00Vol% C4H8O2	ca.69%LEL	ca.31%LEL	ca.41%LEL
		0,35Vol% C9H20	ca.65%LEL	ca.31%LEL	ca.41%LEL
		2,20Vol% CH4	= 50%LEL	ca.26%LEL	ca.35%LEL
		0,75Vol% C4H8O	ca.41%LEL	ca.22%LEL	ca.28%LEL
		1,25Vol% C3H6O	ca.26%LEL	ca.16%LEL	ca.22%LEL
		0,50Vol% C7H8	ca.26%LEL	ca.16%LEL	ca.22%LEL
					ca.26%LEL
Expected lifetime:	6 years				

MK347-5 Electrochemical sensor for nitrogen monoxide NO^[#]

Detection range:	0 .. 100ppm	
Resolution/Tolerance band:	1ppm / ±3ppm	
Response time:	t ₅₀ : < 15s	t ₉₀ : < 40s
Pressure	80...120 kPa:	max. ±1ppm or ±7% of display (referred to 100 kPa)
Humidity	15%...90% r.h.:	max. ±1ppm or ±7% of display (referred to 50% r.h.)
Temperature	-20...+40(50)°C:	max. ±2(4)ppm or ±7% of display (referred to 20°C)
Cross sensitivities:	NO ₂ <30%; H ₂ S≈10%; CO:0%; SO ₂ :0%; (*1)	
Expected lifetime:	2...3 years	
Einlaufzeit:	3 minutes up to 1 day – depending on the time the detector had been turned off	

MK348-5 Electrochemical sensor for nitrogen dioxide NO₂^[#]

Detection range:	0 .. 30ppm	
Resolution/Tolerance band:	0,2ppm / ±0,6ppm	
Response time:	t ₅₀ : < 10 s	t ₉₀ : < 30 s
Pressure	80...120 kPa:	max. ±0.3ppm or ±5% of display (referred to 100 kPa)
Humidity	15%...90% r.h.:	max. ±0.3ppm or ±5% of display (referred to 50% r.h.)
Temperature	-20...+50°C:	max. ±0.3ppm or ±5% of display (referred to 20°C)
Cross sensitivities:	Cl ₂ ≈100%; H ₂ S≈-8%; CO:0%; NO:0%; SO ₂ :0% (*1)	
Expected lifetime:	3 years	

MK353-5 Electrochemical sensor for phosphine PH₃ ^[#]	
Detection range:	0 .. 10ppm
Resolution/Tolerance band:	0,05ppm / ±0,05ppm
Response time:	t ₅₀ : < 20s t ₉₀ : < 60s
Pressure 80...120 kPa:	max. ±0.05ppm or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±0.05ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.05ppm or ±10% of display (referred to 20°C)
Cross sensitivities ^[#] :	SiH ₄ :90%; GeH ₄ :90%; AsH ₃ :65%; B ₂ H ₆ :35%; SO ₂ :20%; CO:0,5%; H ₂ :0,1%; (*1)
Expected lifetime:	2...3 years

MK369-6 / -5 Electrochemical sensors for carbon monoxide CO	
Detection range:	5 .. 500ppm (300ppm ^[#]) zero point drift ≤10ppm
Resolution/Tolerance band:	1ppm / ±3ppm
Response time:	t ₅₀ : < 20 s t ₉₀ : < 50 s t ₁₀ : < 50 s (decay time) The sensor used during high concentrations beyond the upper detection range for several minutes, a decaying zero point in CO in fresh air is certain.
Pressure (70)90...110(130) kPa:	max. ±1ppm or ± 2(8)% of display (referred to 100 kPa)
Humidity 15%...95% r.h.:	max. ±1ppm or ± 2% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+40(55)°C:	max. ±3[6]ppm or ±10% of display (referred to 20°C)
Long term stability per month:	max. ±1ppm or ±1% of display (laboratory conditions)
Cross sensitivities:	H ₂ S<±3%; C ₂ H ₄ :60%; NO:35%; NO ₂ <10%; H ₂ <7%; SO ₂ =0% (*1)
Expected lifetime:	2...3 years

MK379-5 Electrochemical sensor for Ethylen oxide C₂H₄O ^[#]	
Detection range:	0 .. 20ppm
Resolution/Tolerance band:	0,1ppm / ±0,3ppm
Response time:	t ₅₀ : < 30s t ₉₀ : < 120s
Pressure 80...120kPa:	max. ±1ppm or ±15% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±2ppm or ±15% of display (referred to 50% r.h.)
Temperature -(20)0...+40[50]°C:	max. ±1[2]ppm or ±15(20)% of display (referred to 20°C)
Cross sensitivities:	CO≈40%; CH ₄ O≈150%; C ₂ H ₂ ≈125%; CH ₂ O≈120%; CH ₄ S≈100%; C ₂ H ₄ ≈80%; C ₂ H ₆ O≈55%; C ₄ H ₁₀ O≈40%; C ₇ H ₈ ≈20%; MEK≈10%; and others
Expected lifetime:	2...3 years
Warm-up time:	4 minutes up to 7 days – depending on the time the detector had been turned off

MK380-5 Electrochemical sensor for carbon monoxide CO and hydrogen sulfide H₂S (COSH) ^[#]	
Detection range:	0 .. 25%Vol
Resolution:	1ppm CO and 0,5ppm H ₂ S
Tolerance band:	±3ppm CO and ±1,5ppm H ₂ S
Response time:	t ₅₀ : < 20 s t ₉₀ : < 50 s
Pressure 80...120 kPa:	max. ±3(1)ppm or ±7(10)% CO (H ₂ S) reading (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±3(1)ppm or ±7(10)% CO (H ₂ S) reading (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±3(1)ppm or ±15(10)% CO (H ₂ S) reading (referred to 20°C)
Cross sensitivities CO reading:	H ₂ S: 0...40%; H ₂ ≈20%; SO ₂ <20%; NO ₂ <2%; NO<0.3%; Cl ₂ : 0% (*1)
Cross sensitivities H ₂ S reading:	CO<2%; NO ₂ ≈-20%; SO ₂ : 8...20%; NO<3%; H ₂ : 0.03%; Cl ₂ :0% (*1)
Expected lifetime:	3 years

MK383-5 Electrochemical sensor for oxygen O₂ ^[#]	
Detection range:	0 .. 25%Vol
Resolution/Tolerance band:	0,1Vol.% / ±0,3Vol.%
Response time:	t ₂₀ : < 6 s t ₉₀ : < 20 s
Pressure 80...120 kPa:	max. ±0.2Vol.% or ±2.5% of range (referred to 100 kPa)
Humidity 0%...90% r.h.:	max. ±0.2Vol.% or ±2.5% of range (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.5Vol.% or ±2.5% of display (referred to 20°C)
Expected lifetime:	2 years in air

MK390-5 Electrochemical sensor for chlorine Cl₂ ^[#]	
Detection range:	0 .. 10ppm
Resolution/Tolerance band:	0,1ppm / ±0,1ppm
Response time:	t ₅₀ : < 10s t ₉₀ : < 30s
Pressure 80...120 kPa:	max. ±0.2ppm or ±10% of display (referred to 100 kPa)
Humidity 10%...95% r.h.:	max. ±0.2ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.2ppm or ±10% of display (referred to 20°C)
Cross sensitivities:	ClO ₂ :50%; F ₂ :40%; NO ₂ :20%; O ₃ :20%; SO ₂ :18%; CO ₂ :0%; CO:0%; H ₂ S:0%; H ₂ :0% (*1)
Expected lifetime:	2...3 years

MK392-5 Electrochemical sensor for Hydrogen chloride HCl ^[#]	
Detection range:	0 .. 30ppm
Resolution/Tolerance band:	0,2ppm / ±0,4ppm
Response time:	t ₅₀ : < 30s t ₉₀ : < 90s
Pressure 80...120 kPa:	max. ±1ppm or ±10% of display (referred to 100 kPa)
Humidity 10%...95% r.h.:	max. ±1ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±1ppm or ±10% of display (referred to 20°C)
Cross sensitivity:	AsH ₃ :350%; PH ₃ :300%; H ₂ S:65%; NO:45%; SO ₂ :40%; HCN:35%; Cl ₂ :6%; NO ₂ :3%; NH ₃ :0.1%; CO:0%; CO ₂ :0%; H ₂ :0%; (*1)
Expected lifetime:	2...3 years

MK393-5 Electrochemical sensor for ammonia NH₃ ^[#]	
Detection range:	0 .. 200ppm
Resolution/Tolerance band:	1ppm / ±3ppm
Response time:	t ₅₀ : < 20s t ₉₀ : < 60s
Pressure 80...120 kPa:	max. ±1ppm or ±10% of display (referred to 100 kPa)
Humidity 10%...95% r.h.:	max. ±1ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±1(2)ppm or ±10(20)% of display (referred to 20°C)
Cross sensitivities:	H ₂ S:10%; CO:0%; CO ₂ :0%; H ₂ :0%; (*1)
Expected lifetime:	2...3 years
MK396-5 Electrochemical sensor for hydrogen H₂ ^[#] (*2)	
Detection range:	0 .. 2000ppm
Resolution/Tolerance band:	2ppm / ±50ppm
Response time :	t ₅₀ : <30 s t ₉₀ : <90 s
Pressure 800...120 kPa:	max. ±10ppm or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±10ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±20ppm or ±20% of display (referred to 20°C)
Cross sensitivities:	C ₂ H ₄ ≈80%; NO≈35%; HCN≈30%; CO<20%; H ₂ S<20%; NO ₂ :0%; SO ₂ :0%; Cl ₂ :0%; HCl:0% (*1)
Expected lifetime:	2...3 years
MK399-6 Electrochemical sensor for ammonia NH₃ ^[#]	
Detection range:	0 .. 100ppm
Resolution/Tolerance band:	5ppm / ±10ppm
Response time:	t ₅₀ : < 20s t ₉₀ : < 90s
Pressure 80...120 kPa:	max. ±5ppm or ±10% of display (referred to 100 kPa)
Humidity 10%...95% r.h.:	max. ±5ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±5ppm or ±10% of display (referred to 20°C)
Cross sensitivities:	NO ₂ ≈65%, H ₂ S≈60%, Cl ₂ ≈20%, SO ₂ ≈-10%, CO=NO=H ₂ =0% (*1)
Expected lifetime:	2...3 years
MK402-5 Electrochemical sensor for hydrogen H₂ ^[#] (*2)	
Detection range:	0 .. 1.00%Vol
Resolution/Tolerance band:	0,01Vol.% / ±0,02Vol.%
Response time:	t ₅₀ : <40 s t ₉₀ : <70 s
Pressure 80...120 kPa:	max. ±0.01Vol% or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±0.01Vol% or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.02Vol% or ±20% of display (referred to 20°C)
Cross sensitivities:	NO ₂ :~400%; CO:150%; H ₂ S:20%; C ₂ H ₄ :ja; NH ₃ :0%; CO ₂ :0%; Cl ₂ :0%; SO ₂ :0%; HCN:0% (*1)
Expected lifetime:	2...3 years
MK403-5 Electrochemical sensor for hydrogen H₂ ^[#] (*2)	
Detection range:	0 .. 4.00%Vol
Resolution/Tolerance band:	0,01Vol.% / ±0,02Vol.%
Response time:	t ₅₀ : <40 s t ₉₀ : <60 s
Pressure 80...120 kPa:	max. ±0.01Vol% or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±0.01Vol% or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.02Vol% or ±25% of display (referred to 20°C)
Cross sensitivities:	H ₂ S:220%; C ₂ H ₄ :ja; NH ₃ :0%; CO ₂ :0%; CO:0%; Cl ₂ :0%; HCN:0%; NO:0%; NO ₂ :0% (*1)
Expected lifetime:	2...3 years
MK404-5 Electrochemical sensor for Silane SiH₄ ^[#]	
Detection range:	0 .. 40ppm
Resolution/Tolerance band:	0,1ppm / ±0,4ppm
Response time:	t ₅₀ : < 10s t ₉₀ : < 60s
Pressure 80...120 kPa:	max. ±0.1ppm or ±10% of display (referred to 100 kPa)
Humidity 20%...95% r.h.:	max. ±0.1ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+30(40)°C:	max. ±0.2(0.5)ppm or ±10% of display (referred to 20°C)
Cross sensitivities:	PH ₃ :130%; AsH ₃ :100%; B ₂ H ₆ :48%; H ₂ S:35%; SO ₂ :20%; NO ₂ :~20%; HCN:3%; NH ₃ :0%; CO ₂ :0%; CO:0%; Cl ₂ :0%; H ₂ :0%; HCl:0%; (*1)
Expected lifetime:	2 years
MK409-5 Electrochemical sensor for Hydrogen cyanide HCN ^[#]	
Detection range:	0 .. 50ppm
Resolution/Tolerance band:	0,5ppm / ±1,5ppm
Response time:	t ₅₀ : < 25s t ₉₀ : < 60s
Pressure 80...120 kPa:	max. ±0.5ppm or ±10% of display (referred to 100 kPa)
Humidity 10%...95% r.h.:	max. ±0.5ppm or ±10% of display (referred to 50% r.h.)
Temperature -20...+50°C:	max. ±0.5ppm or ±15% of display (referred to 20°C)
Cross sensitivities:	NO ₂ ≈-70%; NO≈-5%; H ₂ S≈0...200% (according to filter saturation); CO=CO ₂ =H ₂ =0% (*1)
Expected lifetime:	2 years

MK427-5 Electrochemical sensor for oxygen O₂	
Detection range:	0 .. 25.0%Vol
Resolution/Tolerance band:	0,1Vol.% / ±0,3Vol.%
Response time:	t ₂₀ : <8 s t ₉₀ : <25 s
Pressure (70)80...130 kPa:	max. ±0.4(0.6)Vol.% or ±2(3)% of range (referred to 100 kPa)
Humidity 0%...95% r.h.:	max. ±0.5Vol.% or ±2.5% of range (referred to 50% r.h. @ 20°C)
Temperature (-20)-10...+55°C:	max. ±0.5(0.8)Vol.% or ±2.5(4.0)% of display (referred to 20°C)
Expected lifetime:	3 years in air
MK429-5/-6 Electrochemical sensor for hydrogen sulfide H₂S	
Detection range:	0.2 .. 100ppm (500ppm ^[#]) Zero point drift < 0.4ppm
Resolution	0,2ppm (0,5ppm)
Tolerance band:	±1,0ppm
Response time:	t ₅₀ : <15 s t ₉₀ : <30 s (decay time)
Pressure 70...130 kPa:	max. ±0.2ppm or ±5% of display (referred to 100 kPa)
Humidity 5%...95% r.h.:	max. ±0.2ppm or ±2% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+40(55)°C:	max. ±0.2ppm or ±5(16)% of display (referred to 20°C)
Long term stability per month:	max. ±0.2ppm or ±2% of display (laboratory condition)
Cross sensitivities:	SO ₂ ≈20%; NO ₂ ≈-20%; CO<1%; NO<0.2%; H ₂ <0.1%; (*1)
Expected lifetime:	3 years
MK440-5/-6 Electrochemical sensor for sulfur dioxide SO₂ ^[#]	
Detection range:	0...10ppm (50ppm)
Resolution/Tolerance band:	0,1ppm / ±0,2ppm
Response time:	t ₅₀ < 10sec t ₉₀ < 30sec
Pressure 80...120kPa:	max. ±0,2ppm or ±5% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±0,3ppm or ±3% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+50°C:	max. ±0,3ppm or ±5% of display (referred to 20°C)
Cross sensitivities:	C ₂ H ₂ <300%; NO ₂ <-170%; C ₂ H ₄ <90%; HCN<50%; Cl ₂ <-40%; NO<10%; H ₂ S<0,4%; CO<0,4%; H ₂ <0,3%; NH ₃ =0%; (*1)
Expected lifetime:	3 years
MK443-5/-6 Electrochemical sensor für carbon monoxide CO ^[#]	
Detection range:	3...500ppm (2000ppm)
Resolution/Tolerance band:	1ppm / ±3ppm
Response time:	t ₅₀ < 10sec t ₉₀ ≤ 30sec t ₁₀ < 30sec
Pressure 80...120kPa:	max. ±3ppm or ±10% of display (referred to 100 kPa)
Humidity 15%...95% r.h.:	max. ±3ppm or ±5% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+40(55)°C:	max. ±3ppm oder ±5(10)% of display (referred to 20°C)
Cross sensitivities:	C ₂ H ₄ ≈100%; C ₂ H ₂ ≈90%; H ₂ <30%(typ.15%); NO<20%; Cl ₂ <7%; C ₂ H ₆ O=0,5%; SO ₂ =NH ₃ =H ₂ S=0% (*1)
Expected lifetime:	3 years
MK445-5/-6 Electrochemical sensor for hydrogen sulfide H₂S ^[#]	
Detection range:	0,2...100ppm (500ppm)
Resolution/Tolerance band:	0,1ppm (0,5ppm) / ±0,5ppm (±1,0ppm)
Response time:	t ₅₀ < 10sec t ₉₀ < 30sec t ₁₀ < 30sec
Pressure 80...120kPa:	max. ±0,2ppm or ±5% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±0,2ppm or ±5% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+40(55)°C:	max. ±0,2ppm or ±5(10)% of display (referred to 20°C)
Cross sensitivities:	NO ₂ <10%; CO<2%; NO<1%, CO ₂ =SO ₂ =Cl ₂ =NH ₃ =C ₂ H ₄ =0% low cross sensitivity to methanol (*1)
Expected lifetime:	3 years
MK453-5 Electrochemical sensor for ammonia NH₃ ^[#]	
Detection range:	0...200ppm
Resolution/Tolerance band:	1ppm / ±3ppm
Response time:	t ₉₀ < 45sec
Pressure 80...120kPa:	max. ±1ppm or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±1ppm or ±10% of display (referred to 50% r.h. @ 20°C)
Temperature (-20)10...+50°C:	max. ±1(2)ppm or ±15(20)% of display (referred to 20°C)
Cross sensitivities:	H ₂ S≈120%; NO ₂ ≈-100%; SO ₂ ≈30%; CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)
Expected lifetime:	2...3 years
MK454-5 Electrochemical sensor for ammonia NH₃ ^[#]	
Detection range:	0...1000ppm
Resolution/Tolerance band:	5ppm / ±10ppm
Response time:	t ₉₀ < 60sec
Pressure 80...120kPa:	max. ±5ppm or ±10% of display (referred to 100 kPa)
Humidity 15%...90% r.h.:	max. ±5ppm or ±10% of display (referred to 50% r.h. @ 20°C)
Temperature -20...+55°C:	max. ±10ppm or ±20% of display (referred to 20°C)
Cross sensitivities:	H ₂ S≈140%; NO ₂ ≈-100%; SO ₂ ≈30%; CO=NO=CO ₂ =H ₂ =C ₂ H ₆ O=0% (*1)
Expected lifetime:	2...3 years

zu (*1): Displayed value with reference to the supplied gas concentration in the range of ch von WEL (TLV)
zu (*2): Not approved for LEL monitoring for applications of primary explosion protection

Alarm Thresholds – Standard Setpoints

Standard setting of alarm thresholds for toxic gases without exposition alarm

Detection range	Alarm 1	Alarm 2	STEL	TWA
0 ... 20ppm C ₂ H ₄ O	2ppm (*1)	4ppm	-	-
0 ... 500/2000ppm C ₄ H ₈	100ppm	200ppm	-	-
0 ... 300/500/1000/2000ppm CO	30ppm	60ppm	-	-
0 ... 5,0Vol.% CO ₂	0.5Vol.%	1.0Vol.%	-	-
0 ... 10ppm Cl ₂	0,5ppm (*1)	1ppm (*1)	-	-
0 ... 100/500ppm H ₂ S	10ppm	20ppm	-	-
0 ... 30ppm HCl	5ppm	10ppm	-	-
0 ... 50ppm HCN	10ppm	20ppm	-	-
0 ... 200/1000ppm NH ₃	50ppm	100ppm	-	-
0 ... 100ppm NO	25ppm	50ppm	-	-
0 ... 30ppm NO ₂	5ppm	10ppm	-	-
0 ... 10ppm PH ₃	0,3ppm (*1)	0,4ppm (*1)	-	-
0 ... 40ppm SiH ₄	5ppm	10ppm	-	-
0 ... 10ppm SO ₂	2ppm	4ppm	-	-

at (*1): WEL monitoring cannot be recommended with the available sensor technology

Standard setting of alarm thresholds for toxic gases with exposition alarm following to TRGS900

Messbereich	Alarm 1	Alarm 2	STEL (15')	TWA (8h)
0 ... 20ppm C ₂ H ₄ O	2ppm	6ppm	4ppm	2ppm
0 ... 500/2000ppm C ₄ H ₈	100ppm	400ppm	200ppm	100ppm
0 ... 300/500/1000/2000ppm CO	30ppm	120ppm	60ppm	30ppm
0 ... 5,0Vol.% CO ₂	0,5Vol.%	2,0Vol.%	1,0Vol.%	0,5Vol.%
0 ... 10ppm Cl ₂	0,5ppm	1ppm	0,5ppm	0,5ppm
0 ... 100ppm H ₂ S	5ppm	20ppm	10ppm	5ppm
0 ... 30ppm HCl	5ppm	10ppm	5ppm	5ppm
0 ... 50ppm HCN	10ppm	20ppm	10ppm	10ppm
0 ... 200ppm NH ₃	20ppm	80ppm	40ppm	20ppm
0 ... 100ppm NO	25ppm	50ppm	35ppm	25ppm
0 ... 30ppm NO ₂	5ppm	10ppm	5ppm	5ppm
0 ... 10ppm PH ₃	0,3ppm (*1)	0,4ppm	0,2ppm	0,1ppm
0 ... 40ppm SiH ₄	5ppm	15ppm	10ppm	5ppm
0 ... 10ppm SO ₂	1ppm	2ppm	1ppm	1ppm

at (*1):WEL monitoring cannot be recommended with the available sensor technology.

Standard setpoints of alarm thresholds for combustible gases and oxygen

Detection range	Alarm 1	Alarm 2	Alarm 3
0 ... 25Vol.% O ₂	19.0Vol.% (↓)	17.0Vol.% (↓)	23.0Vol.% (↑)
0 ... 2000ppm H ₂ (*2)	1000ppm	1500ppm	2000ppm
0 ... 1.0/4.0Vol.% H ₂ (*2)	0.20Vol.%	0.40Vol.%	0.60Vol.%
0 ... 5.0Vol.% CH ₄	1.00Vol.%	2.00Vol.%	3.00Vol.%
0 ... 100%LEL CH ₄ (*3)	20.0%LEL	40.0%LEL	60.0%LEL

at (*2): Not approved for LEL monitoring in applications subject to primary explosion protection.

at (*3): or another one of the following combustible gases and vapours

LEL values as per IEC 79-20 resp. data base CHEMSAFE	
4.0%Vol. H ₂ (hydrogen)	6,0%Vol. CH ₄ O (methanol)
4.4%Vol. CH ₄ (methane)	3.1%Vol. C ₂ H ₆ O (ethanol)
2.3%Vol. C ₂ H ₂ (acetylene)	2.5%Vol. C ₃ H ₆ O (acetone)
2.3%Vol. C ₂ H ₄ (ethylene)	3,1%Vol. C ₃ H ₆ O ₂ (methylacetate)
2.4%Vol. C ₂ H ₆ (ethane)	2.7%Vol. C ₃ H ₆ O ₂ (ethyl formate ETF)
1.7%Vol. C ₃ H ₈ (propane)	2.0%Vol. C ₃ H ₈ O (iso-propanol)
1.4%Vol. C ₄ H ₁₀ (butane)	1.5%Vol. C ₄ H ₈ O (methyletylketone MEK)
1.1%Vol. C ₅ H ₁₂ (pentane)	2.0%Vol. C ₄ H ₈ O ₂ (ethylacetate)
1.0%Vol. C ₆ H ₁₄ (n-hexane)	1.4%Vol. C ₃ H ₁₀ O (n-butanol)
0,85%Vol. C ₇ H ₁₆ (heptane)	1.2%Vol. C ₆ H ₁₂ O (methylisobutylketone MIBK)
0.7%Vol. C ₉ H ₂₀ (n-nonane)	1.0%Vol. C ₇ H ₈ (toluene)

Technical Data

Type:	G460		
Detection principle:	Electrochemical (EC):	for toxic gases and oxygen	
	Photo-ionisation (PID):	for toxic combustible vapours (in ppm range)	
	Cat. combustion (CC):	for combustible gases and vapours (up to 100 %LEL)	
	Infrared (IR):	for combustible gases and vapours and carbon dioxide	
Detection ranges:	see "Sensor Types and Detection Ranges"		
Response time t_{90}:	see "Sensor Specification"		
Expected sensor life:	2...6 years - see "Sensor Specification"		
Gas supply:	Diffusion with a flow velocity of 0 .. 6 m/s or Pump by means of attachable electrical sampling pump G400-MP2 ^[1]		
Display:	Illuminated LCD full graphic display, automatical size adjustment for optimal readout, display of battery capacity, gas concentration as instantaneous and peak value		
Alarm:	Depending on gas 3 or 2 instantaneous and 2 dosimeter alarms, battery alarm. Visual and audible warning and display indication, colouring of display depending on alarm status (orange/red) Buzzer: 103 dB(A) (reducible to 90 dB(A))		
Zeropoint and sensitivity calibration:	Manually or automatically with calibration program or test gas supply by using "Smart Cap" or "Smart Charger Cap" with 0.5..0.6 l/min.		
Power supply:	<ol style="list-style-type: none"> NiMH rechargeable module A21 (black housing), 2100mAh rechargeable NiMH rechargeable module F25 (black housing), 2500mAh rechargeable $I_m = 600\text{mA}$ (max. charging current) $U_m = 6\text{V DC}$ (max. voltage) or Alkaline battery module (grey housing), not rechargeable with 2x AA Mignon 1.5V Type: DURACELL PROCELL MN1500 LR6 AA or INDUSTRIAL^{BY} DURACELL ID1500 AA (LR6) 		
Operational time ^(*1)			
	NiMH-II A21:	approx. 9h (EC+CC); approx. 7h (EC+IR+CC); approx. 8h (EC+PID+CC); approx. 6h (EC+PID+IR+CC);	approx. 17h (EC+CC _{CH4}); approx. 11h (EC+IR+CC _{CH4}); approx. 12h (EC+PID+CC _{CH4}); approx. 8h (EC+PID+IR+CC _{CH4});
	NiMH F25:	approx. 11h (EC+CC); approx. 7-8h (EC+IR+CC); approx. 9h (EC+PID+CC); approx. 6h (EC+PID+IR+CC); (EC+PID+IR)	approx. 120h (EC) approx. 25h (EC+IR) approx. 33h (EC+PID) approx. 14h (EC+PID+IR) approx. 20h (EC+CC _{CH4}); approx. 12h (EC+IR+CC _{CH4}); approx. 14h (EC+PID+CC _{CH4}); approx. 10h (EC+PID+IR+CC _{CH4}); approx. 17h
	Alkaline:	approx. 8h (EC+CC); approx. 5h (EC+IR+CC); approx. 6h (EC+PID+CC);	approx. 14h (EC+CC _{CH4}); approx. 6h (EC+IR+CC _{CH4}); approx. 9h (EC+PID+CC _{CH4});
Climate conditions:			
	for operation	-20...+50°C 5...95% r. h. 70...130 kPa	
	for storage	-25...+60°C 5...95% r. h. 70...130 hPa (recommended 0...+30°C)	

To be continued on the next page

Continuation of "technical data"

Enclosure:			
Material:	Rubberized plastic		
Dimensions:	75 x 110 x 55 mm (W x H x D)		
Weight:	approx. 350 g (depending on sensor configuration)		
Protection:	IP67		
Approvals and Certificates:			
Labelling and ignition protection:	⊕ I I2G	Ex ia de IIC T4 Gb	-20°C ≤ Ta ≤ +50°C for NiMH-II (black)
		Ex ia de IIC T3 Gb	-20°C ≤ Ta ≤ +50°C for NiMH (black)
		Ex ia de IIC T4/T3Gb	-20°C ≤ Ta ≤ +45°C/+50°C for Alkaline (grey)
	⊕ I M1	Ex ia IIC Ma	-20°C ≤ Ta ≤ +50°C for NiMH, NiMH-II (black)
EC-Type Examination Certificate:	BVS 06 ATEX E 017 X	(for measuring function and electronic EX-protection) (s. chapter "Application and Purpose")	
Type Examination Certificate:	PFG 09 G 001	(for measuring function) (s. chapter "Application and Purpose")	
Electro-Magnetic Compatibility:	DIN EN 50270 : 2006	Radio shielding:	Type class I
		Interference resistance:	Type class II

(*1): The operational time will be decreased by hitting keys (display illumination & lights) and by alarms being triggered.


**Worldwide Supplier
of Gas Detection Solutions**




GfG Gesellschaft für Gerätebau mbH
 Klönnestr. 99 – D-44143 Dortmund
 Phone: +49 (0)231 – 564 00-0
 Telefax: +49 (0)231 – 51 63 13
 E-Mail: info@gfg.biz
 Internet: www.gasdetection.biz

205-003.34_OM_G460.doc, Edition: 25th October 2017
 We reserve the right of modification, Firmware Version 3.44

EC-Type Examination Certificate





Translation
6th Supplement

(Supplement in accordance with Directive 94/9/EC Annex III number 6)

to the EC-Type Examination Certificate
BVS 06 ATEX E 017 X

Equipment: Gas detector type G450 and type G460
Manufacturer: GFG Gesellschaft für Gerätebau mbH
Address: 44143 Dortmund, Germany

Description

The gas detectors type G450 and type G460 can be modified according to the descriptive documents as mentioned in the pertinent test and assessment report.


In Group I, the gas detector type G460 has to be used only with the NiMH battery pack or the NiMH-II battery pack.


The marking of the gas detectors type G450 and type G460 was modified according to the used standards.

The Essential Health and Safety Requirements of the modified equipment are assured by compliance with:


EN 60079-0:2009	General requirements
EN 60079-1:2007	Flameproof enclosure 'd'
EN 60079-7:2007	Increased safety 'c'
EN 60079-11:2007	Intrinsic safety 'i'
EN 50303:2000	Equipment for Group I Category M1

The marking of the equipment shall include the following:

for type G450
 **II 2G Ex ia d IIC T4/T3 Gb**
I M2 Ex ia d I Mb

for type G460
 **II 2G Ex ia de IIC T4/T3 Gb**
I M1 Ex ia I Ma (Only with battery pack NiMH or NiMH-II)

Page 1 of 1 to BVS 06 ATEX E 017 X / N6
 This certificate may only be reproduced in its entirety and without change.
 DEKRA EXAM GmbH | Dienstleistungsstr. 9 | 44809 Bochum | Germany | Phone: +49 234 3696-110 | Fax: +49 234 3696-110 | E-mail: zs-exam@dekra.com
 (until 31.03.2007 EXAM BBG Prüf- und Zertifizierung GmbH)



Special conditions for safe use.

The measurement function for explosion protection is not the subject of this supplement to the EC-Type Examination Certificate.

In Group I, the gas detector type G460 has to be used only with the NiMH battery pack or the NiMH-II battery pack.

Test and assessment report
 BVS PP 06.2017 EG as of 19.11.2010


DEKRA EXAM GmbH
 Bochum, dated 19 November 2010

Signed: Dr. Franz Eickhoff Signed: Günther Schumann


 Certification body Special services unit

We confirm the correctness of the translation from the German original.
 In the case of arbitration only the German wording shall be valid and binding.

44809 Bochum, 19.11.2010
 BVS-Rip/Her / A 20100479
DEKRA EXAM GmbH




 Certification body



 Special services unit

Page 2 of 3 to BVS 06 ATEX E 017 X / N6
 This certificate may only be reproduced in its entirety and without change.
 DEKRA EXAM GmbH | Dienstleistungsstr. 9 | 44809 Bochum | Germany | Phone: +49 234 3696-110 | Fax: +49 234 3696-110 | E-mail: zs-exam@dekra.com
 (until 31.03.2007 EXAM BBG Prüf- und Zertifizierung GmbH)



Parameters

1 Type of protection and ambient temperature range of the complete device type G450 with different combination of individual components:

Type of protection / EPL	Ambient temperature range
Gas detector with NiMH battery pack (marking Ex ia I, Ex ia IIC T3) (colour: black)	-20 °C ≤ T _a ≤ +55 °C -20 °C ≤ T _a ≤ +55 °C
Gas detector with NiMH-II battery pack (marking Ex ia I, Ex ia IIC T4) (colour: black)	-20 °C ≤ T _a ≤ +55 °C -20 °C ≤ T _a ≤ +55 °C
Gas detector with Alkaline battery pack (colour: grey)	-20 °C ≤ T _a ≤ +45 °C -20 °C ≤ T _a ≤ +55 °C -20 °C ≤ T _a ≤ +55 °C

2 Type of protection and ambient temperature range of the complete device type G460 with different combination of individual components:

Type of protection / EPL	Ambient temperature range
Gas detector with NiMH battery pack (marking Ex ia I, Ex ia IIC T3) (colour: black)	-20 °C ≤ T _a ≤ +50 °C -20 °C ≤ T _a ≤ +50 °C
Gas detector with NiMH-II battery pack (marking Ex ia I, Ex ia IIC T4) (colour: black)	-20 °C ≤ T _a ≤ +50 °C -20 °C ≤ T _a ≤ +50 °C
Gas detector with Alkaline battery pack (colour: grey)	-20 °C ≤ T _a ≤ +45 °C -20 °C ≤ T _a ≤ +50 °C

3 NiMH and NiMH-II battery pack:
 Nominal voltage: 2.4 V
 Nominal capacity: 2500 mAh
 Maximum charging voltage: U_{in}
 DC 6 V

4 Alkaline battery pack:
 Nominal voltage: 3 V

The approved Alkaline battery types are listed in the manufacturer instructions of GFG Gesellschaft für Gerätebau mbH.

Page 2 of 3 to BVS 06 ATEX E 017 X / N6
 This certificate may only be reproduced in its entirety and without change.
 DEKRA EXAM GmbH | Dienstleistungsstr. 9 | 44809 Bochum | Germany | Phone: +49 234 3696-110 | Fax: +49 234 3696-110 | E-mail: zs-exam@dekra.com
 (until 31.03.2007 EXAM BBG Prüf- und Zertifizierung GmbH)



Translation
4th Supplement
to the EC-Type Examination Certificate
BVS 06 ATEX E 017 X

(Supplement in accordance with Directive 94/9/EC Annex III number 6)

Equipment: Gas detectors type G450 and G460
Manufacturer: GFG Gesellschaft für Gerätebau mbH
Address: D-44143 Dortmund

Description

The Essential Health and Safety Requirements with respect to the measuring function for explosion protection are assured by application of:

EN 60079-29-1:2007
EN 50271:2001

This supplement to the EC-type examination certificate covers devices with software version 3.31 and infrared-sensors with software version 2.07.

This supplement to the EC-type examination certificate covers the measuring function for methane, propane and n-hexane with the measuring range 0 to 100 % LEL (sensors MK221-0(-)1 and MK211-6(-)7), for propane with the measuring range 0 to 100 % LEL and n-hexane with concentrations up to 60 % LEL (sensors MK227-5 and MK231-5).

Test report

Test report PFG-no. 41300209P dated 30/11/2009

Special conditions for safe use

- The system option "AL latching" shall be set "on".
- After an extreme impact the zero of the sensors shall be checked and, if necessary, adjusted.
- The indications with zero gas and test gas shall be tested before every use.

DEKRA EXAM GmbH
Bochum, dated 30/11/2009

Signed: Müller
Certification body

Signed: Kiesewetter
Special services unit



Translation
Type Examination Certificate

- Gas detectors -
PFG 09 G 001

Equipment: Gas detectors type G450 and type G460
Manufacturer: GFG Gesellschaft für Gerätebau mbH
Address: D-44143 Dortmund

The certification body of DEKRA EXAM GmbH certifies that this equipment has been found to comply with the requirements of the standards or "Berufsgenossenschaftlichen Informationen", respectively,

EN 50104:2002 + A1:2004
EN 45544-1:1999
EN 45544-2:1999
EN 50271:2001
BGI 836 (July 2009)

with regard to the measuring function for oxygen (measurement of oxygen deficiency and enrichment) in the measuring range 0 - 25 % (v/v) (sensors MK381-0(-)5 and MK427-0(-)5), for hydrogen sulphide in the measuring range 0.2 - 100 ppm (sensors MK429-0(-)5) or 0.4 - 100 ppm (sensors MK386-0(-)5), for carbon monoxide in the measuring range 3 - 500 ppm (sensors MK344-0(-)4) or 5 - 500 ppm (sensors MK369-0(-)6 and MK384-0(-)5) and for carbon dioxide in the measuring range 0.02 - 5 % (v/v) (sensors MK231-5 and MK224-5).

This type examination certificate covers equipment with software version 3.31 and infrared-sensors with software version 2.07.

On the basis of DIN EN 45011, this certification includes a type examination. The examination and test results and the design of the equipment are recorded in the test report PFG-Nr. 41300209P.

If the sign "X" is placed after the certificate number, it indicates that the equipment is subject to special conditions for safe use specified in the annex to this certificate.

The manufacturer declares the conformity of the manufactured products with the certified design by marking them with the number of this type examination certificate.

DEKRA EXAM GmbH
Bochum, dated 30. November 2009

Signed: Müller
Certification body

Signed: Kiesewetter
Special services unit



Annex to
Type Examination Certificate
PFG 09 G 001

Description of the gas detector

The gas detection apparatus type G450 and G460 are portable devices for the measurement of combustible gases and vapours mixed with air, of oxygen and of toxic gases.

Devices type G450 can be equipped with a catalytic combustion sensor for the measurement of combustible gases and vapours, a sensor for the measurement of oxygen and two sensors for the measurement of toxic gases.

Devices type G460 can be equipped with a catalytic combustion sensor for the measurement of combustible gases and vapours, a sensor for the measurement of oxygen, two sensors for the measurement of toxic gases and an infrared sensor for the measurement of combustible gases and vapours and/or carbon dioxide.

It is not necessary that all sensors are equipped. A rechargeable NiMH-battery pack serves as power supply.

Type of protection

- II 2 G Ex ia d IIC T4/T3 (type G450)
- II 2 G Ex ia d IIC T4/T3 (type G460)

Special conditions for safe use

Not applicable

Additional Information

- The measuring function of the device for combustible gases and vapours according to directive 94/9/EC is subject of the 4th supplement to the EC-type examination certificate BVS 06 ATEX E 017 X.
- This type examination certificate includes the following accessories:
 - docking station DS 400 (software version 2.20) (part no. 1450401)
 - Calibration cap "Smart Cap" (part no. 1450225)
 - Smart Charger Cap (part no. 1450215)
 - Drop In Charger G400-DIC1 (part no. 1450219)
 - Drop In Charger G400-DIC2 (part no. 1450223)
- The data logger is not subject of this type examination certificate.

Translation

7. Supplement to the EC-Type Examination Certificate

- (1) Equipment and protective systems intended for use in potentially explosive atmospheres - Directive 94/9/EC Supplement accordant with Annex III number 6
- (2) No. of EC-Type Examination Certificate: **BVS 06 ATEX E 017 X**
- (3) Equipment: **Gas detector type G460**
- (4) Manufacturer: **GFG Gesellschaft für Gerätebau mbH**
- (5) Address: **D-44143 Dortmund**
- (6) The design and construction of this equipment and any acceptable variation thereto are specified in the appendix to this supplement.
- (7) The certification body of DEKRA EXAM GmbH, notified body no. 0156, in accordance with Article 9 of the Directive 94/9/EC of the European Parliament and the Council of 23 March 1994, certifies that this equipment has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment and protective systems intended for use in potentially explosive atmospheres, given in Annex II to the Directive. The examination and test results are recorded in the test report PFG-no. 41300209P-NI.
- (8) The Essential Health and Safety Requirements with respect to this measuring function for explosion protection are assured by application of:
EN 60079-29-1:2007
EN 60271:2001
- (9) This supplement to the EC-type examination certificate covers for the gas detector type G460 for use in mines susceptible to firedamp, the measuring function for methane in the measuring ranges 0 to 5 % (v/v) CH₄ (sensor MK211-3) when operated with or without the gas pump G400-MP2. This supplement to the EC-type examination certificate covers gas detector's type G460 with software version 3.44 and gas pumps G400-MP2 with software version 2.04.
- (10) If the sign "X" is placed after the certificate number, it indicates that the equipment is subject to special conditions for safe use specified in the appendix to this certificate.
- (11) This supplement to the EC-Type Examination Certificate relates only to the design examination and tests of the specified equipment in accordance to Directive 94/9/EC. Further requirements of the Directive apply to the manufacturing process and supply of this equipment. These are not covered by this certificate.
- (12) The marking of the gas detector shall include the following:
see 6. supplement to BVS 06 ATEX E 017 X
see 5. supplement to BVS 07 ATEX E 011

The marking of the pump shall include the following:

see 5. supplement to BVS 07 ATEX E 011

DEKRA EXAM GmbH
Bochum, dated 03. August 2012

Signed: Migenda

Certification body

Signed: Kiesevetter

Special services unit

Page 1 of 2 to BVS 06 ATEX E 017 X / NY

This certificate may only be reproduced in its entirety and without change.

DEKRA EXAM GmbH Dimensionalstrasse 9 44809 Bochum Phone +49 234 3696-105 Fax +49 234 3696-110 zs-exam@deka.com

(13) Appendix to

(14) **7. Supplement to the EC-Type Examination Certificate**
BVS 06 ATEX E 017 X

(15) **15.1 Subject and type**

Gas detector type G460 when operated with or without gas pump G400-MP2.

15.2 Description

This supplement to the EC-type examination certificate concerns modifications of hardware and software and use of the apparatus in mines susceptible to firedamp. The equipment can be modified according to the descriptive documents as mentioned in the pertinent test report

15.3 Parameters

See EC-type examination certificate BVS 06 ATEX E 017 X and supplements 1 to 5
See EC-type examination certificate BVS 07 ATEX E 011 and supplements 1 to 5

(16) **Test and assessment report**

PFG-no. 41300209P-NI as of 03.08.2012

EC-type examination certificate BVS 06 ATEX E 017 X and supplements 1 to 5

EC-type examination certificate BVS 07 ATEX E 011 and supplements 1 to 5

(17) **Special conditions for safe use**

The following special properties have to be considered at operation of the gas detector:

- The system option "AL latching" shall be set "on"
- After an extreme impact the zero of the sensors shall be checked and, if necessary, adjusted
- The indications with zero gas and test gas shall be tested before every use.

We confirm the correctness of the translation from the German original.
In the case of arbitration only the German wording shall be valid and binding.

DEKRA EXAM GmbH
44809 Bochum, 03. August 2012
PFG-Kie/Bre

Migenda
Certification body

Kiesevetter
Special services unit

Page 2 of 2 to BVS 06 ATEX E 017 X / NY


This certificate may only be reproduced in its entirety and without change.

DEKRA EXAM GmbH Dimensionalstrasse 9 44809 Bochum Phone +49 234 3696-105 Fax +49 234 3696-110 zs-exam@deka.com

EU Declaration of Conformity GfG Gesellschaft für Gerätebau mbH

G460 MICROTECTOR II

Klönnestraße 99
44143 Dortmund
Tel: +49 (231) 56400-0
Fax: +49 (231) 516313
E-Mail: info@gfg-mbh.com
www.gfg.biz



Edited: 21.06.2007 Amended: 08.08.2017

GfG Gesellschaft für Gerätebau mbH develops produces and sells gas sensors and gas warning devices which are subject to a **quality management system** as per DIN EN ISO 9001.

Subject to supervision by means of a **quality system**, audited by the notified body, DEKRA EXAM GmbH (0158), is the production of electrical apparatus of instrumentation Group I and II, categories M1, M2, 1G and 2G for gas sensors, gas detectors, gas warning systems in types of protection flameproof enclosures, increased safety, encapsulation and intrinsic safety, as well as their measuring function.

The portable detector **G460** complies with directive **2014/34/EU** (ATEX) for devices and protective systems for proper use in potentially explosive atmospheres, directive **2014/30/EU** for electromagnetic compatibility and with directive **2011/65/EU** (RoHS) on the restriction of the use of certain hazardous substances in electrical and electronic equipment.

For electrical explosion protection Labelling		BVS 06 ATEX E 017 X	
⊕ II 2G Ex ia de IIC T4 Gb		-20°C≤Ta≤+50°C	(NiMH-II)
⊕ II 2G Ex ia de IIC T3 Gb		-20°C≤Ta≤+50°C	(NiMH)
⊕ II 2G Ex ia de IIC T4/T3 Gb		-20°C≤Ta≤+45°C/+50°C	(Alkaline)
⊕ I M1 Ex ia I Ma		-20°C≤Ta≤+50°C	(NiMH, NiMH-II)

EC-Type Examination Certificate according to directive 94/9/EG

- General requirements	EN 60079-0	: 2009
- Flameproof enclosure "d"	EN 60079-1	: 2007
- Increased safety "e"	EN 60079-7	: 2007
- Intrinsic safety "i"	EN 60079-11	: 2007
- Group1, category-M1-equipment	EN 50303	: 2000
- Gas detectors - Performance requirements of detectors for flammable gases	EN 60079-29-1	: 2007
- Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen - Requirements and tests for apparatus using software and/or digital technologies.	EN 50271	: 2001

Certified by the notified body with ID number 0158 (DEKRA EXAM, Dinnendahlstraße 9, D-44809 Bochum).

The directive 2014/34/EU is complied considering the following standards:

- General requirements	EN 60079-0	: 2012 +A11 :2013
- Flameproof enclosures "d"	EN 60079-1	: 2014
- Increased safety "e"	EN 60079-7	: 2015
- Intrinsic safety "i"	EN 60079-11	: 2012
- Group1, category-M1-equipment	EN 50303	: 2000

The rating of the danger of ignition was done and documented.

- Gas detectors - Performance requirements of detectors for flammable gases	EN 60079-29-1	: 2007
- Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen - Requirements and tests for apparatus using software and/or digital technologies.	EN 50271	: 2001

The directive 2014/30/EU is complied considering the following standard:

- Electromagnetic compatibility - Electrical apparatus for the detection and measurement of combustible gases, toxic gases or oxygen	EN 50270	: 2006
Emitted interference	Type class 1	
Interference immunity	Type class 2	

The EMC test laboratory EM TEST GmbH in Kamen has tested and certified the electromagnetic compatibility.

The directive 2011/65/EU is complied considering the following standard:

- Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances	EN 50581	: 2012
--	----------	--------

Dortmund, 14 September 2017

.....
QMB B. Siebrecht

ATEX EU-Kon99/Siebrecht